


Mass Spectrum

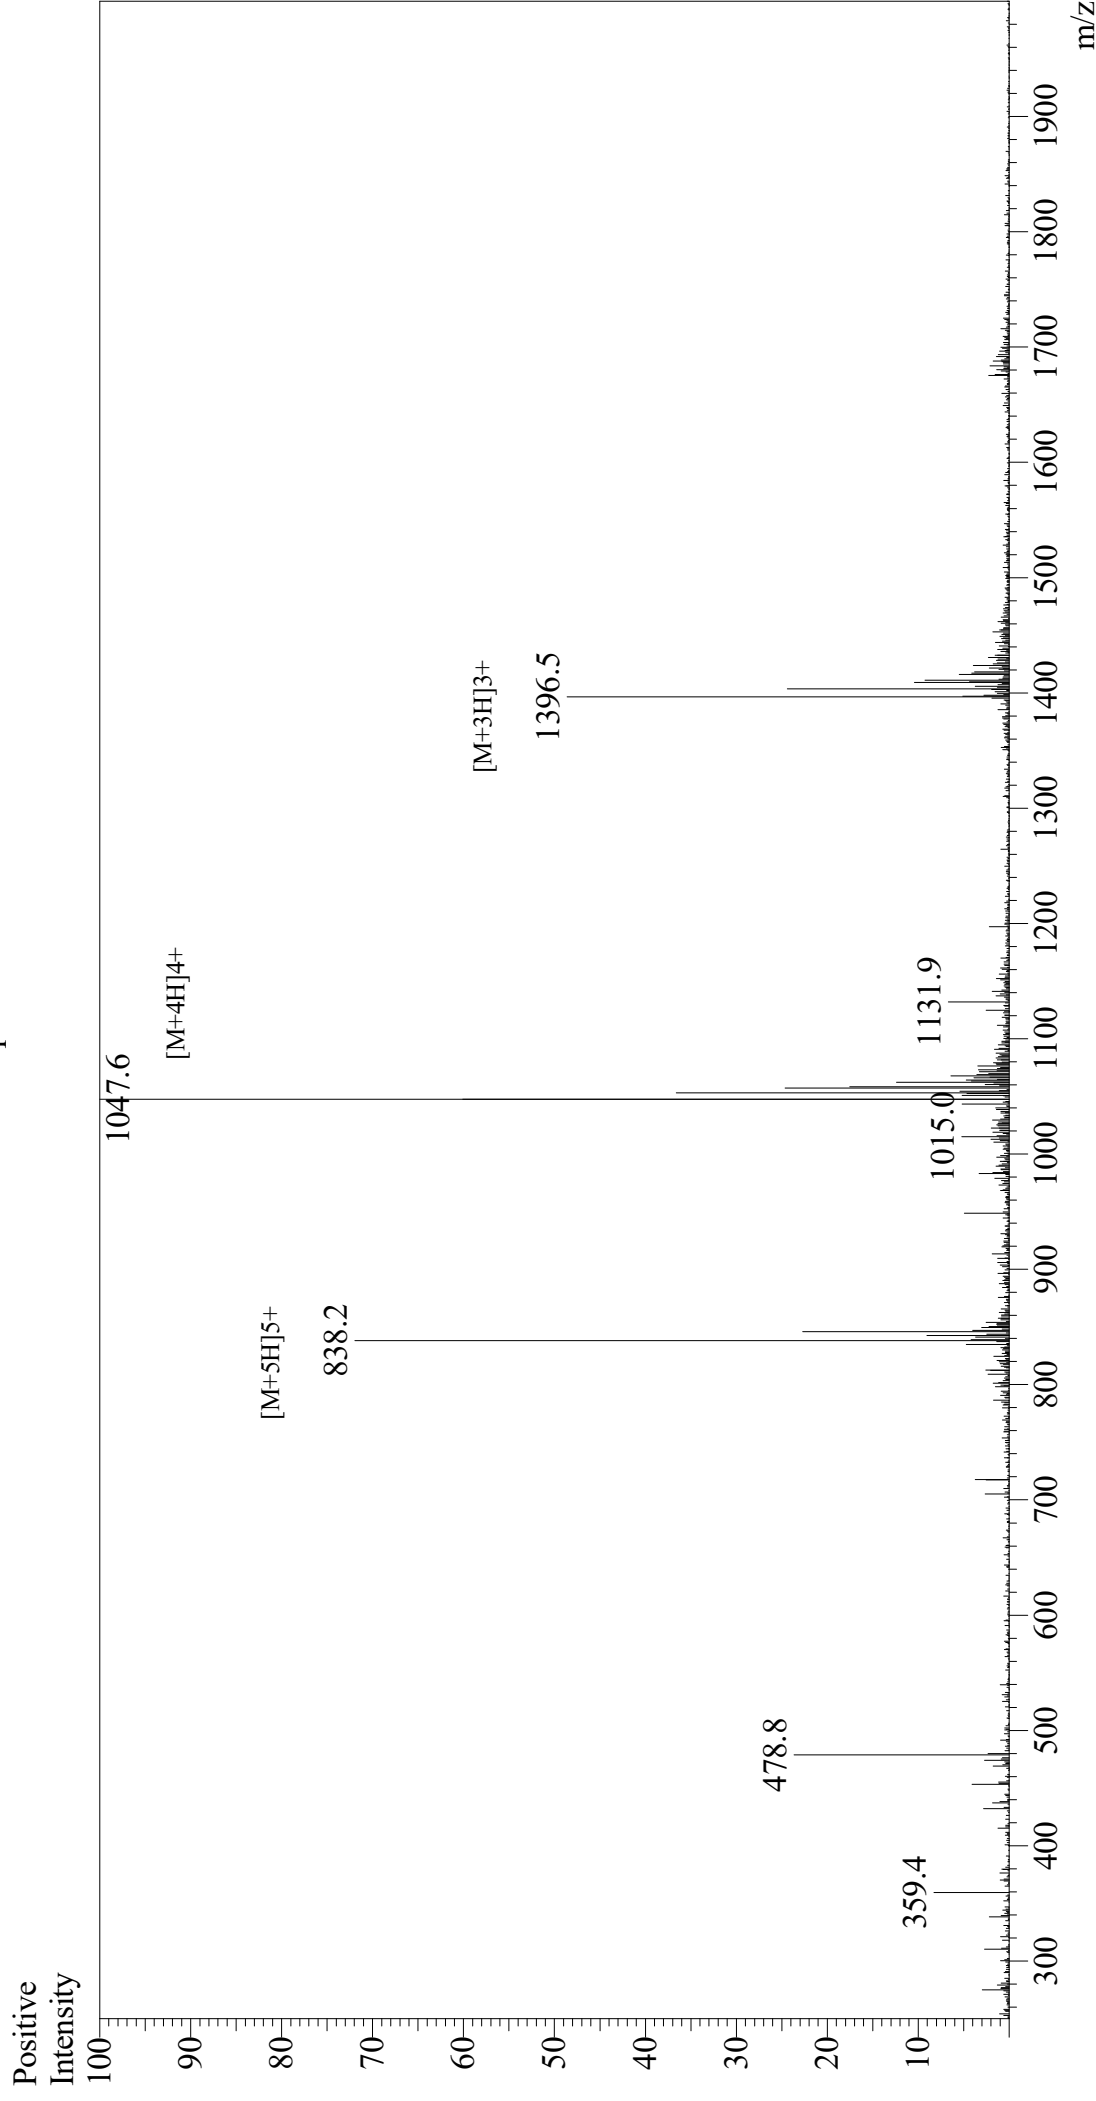

Sample Information

Month-Day Processed : 09/30/21
 Time Processed : 20:47:15
 Injection Volume : 0.4
 Sample Name : Exendin-4
 Cat No. : RP10874
 Lot No. : E9862621I
 Theoretical MW : 4186.66
 Observed MW : 4186.4

Interface

Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Interface Bias : +3.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H2O/50%MeOH