

Sample Name :β-Melanocyte Stimulating Hormone (MSH), human
 Cat No: RP10648
 Lot No : E2539520J
 Time Processed :12:34:57 AM
 Month-Day-Year Processed :10/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
85.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

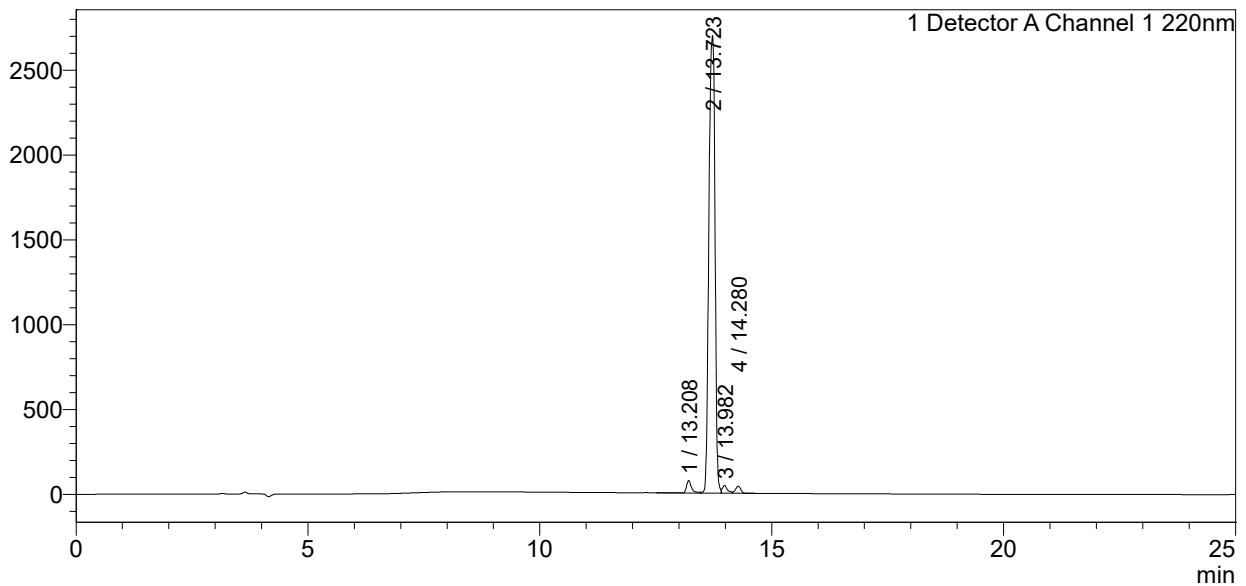

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.208	552631	74289	2.140
2	13.723	24593717	2698008	95.255
3	13.982	344969	46076	1.336
4	14.280	327568	41265	1.269
Total		25818885	2859638	100.000