

Sample Name:Gastric Inhibitory Peptide (GIP), human
 Cat No :RP10795
 Lot No :E0929821E
 Time Processed :1:04:56 AM
 Month-Day-Year Processed :05/26/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

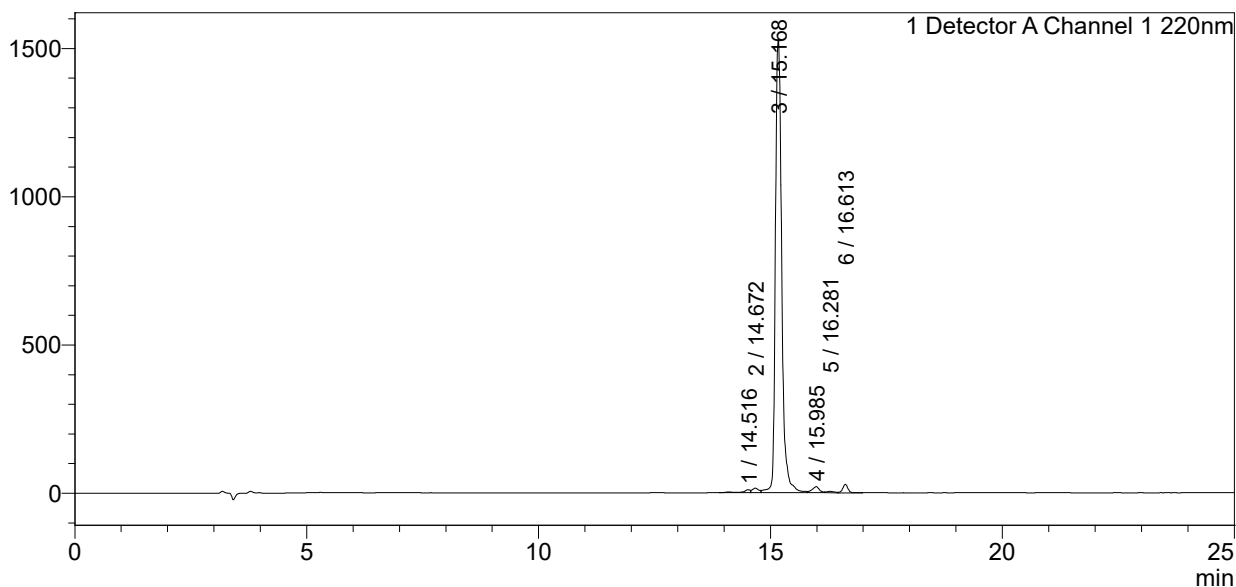

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.516	112144	9817	0.736
2	14.672	142955	15064	0.939
3	15.168	14472691	1531755	95.015
4	15.985	224643	20614	1.475
5	16.281	57037	4563	0.374
6	16.613	222568	28329	1.461
Total		15232038	1610141	100.000