

Sample Name : Somatostatin
Cat. No. : RP10226
Lot. No. : PE5061611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

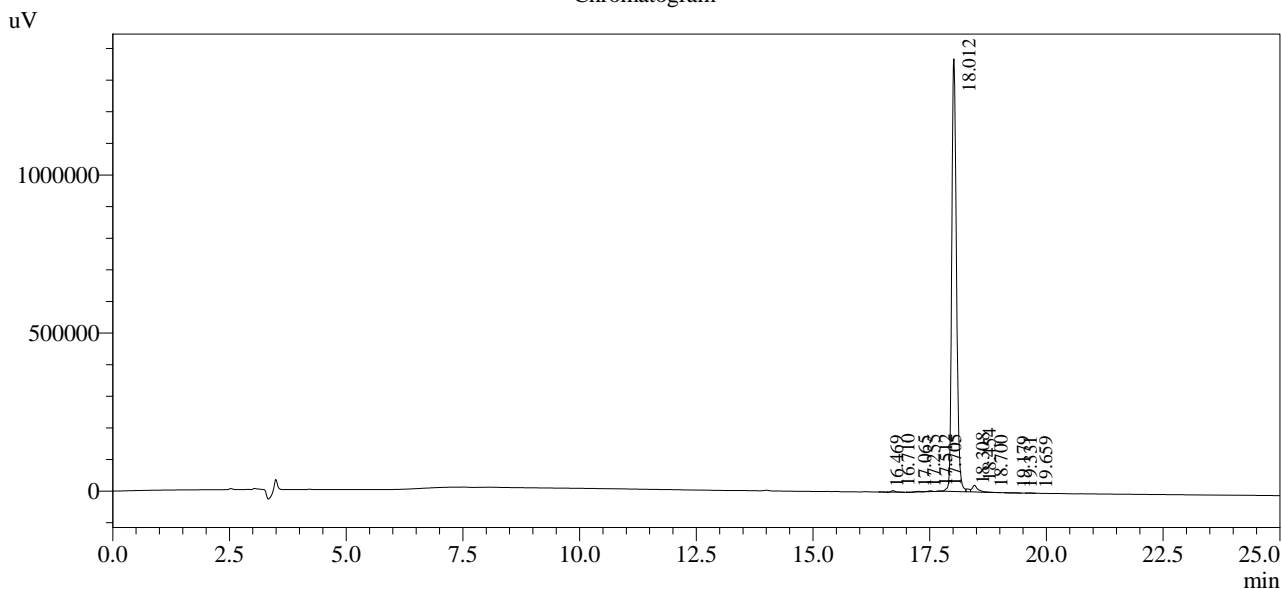

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.469	1400	328	0.014
2	16.710	27938	4508	0.282
3	17.065	717	177	0.007
4	17.255	11809	1827	0.119
5	17.512	17528	2624	0.177
6	17.705	4867	1113	0.049
7	18.012	9597295	1368314	96.919
8	18.308	49861	8933	0.504
9	18.454	172223	20953	1.739
10	18.700	7949	1277	0.080
11	19.179	2785	471	0.028
12	19.331	3988	652	0.040
13	19.659	4027	753	0.041
Total		9902388	1411928	100.000