

Sample Name : N-Formyl-Met-Leu-Phe-Lys
 Cat. No. : RP12958
 Lot. No. : E4883419I
 Time Processed :20:04:38
 Month-Day-Year Processed :09/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

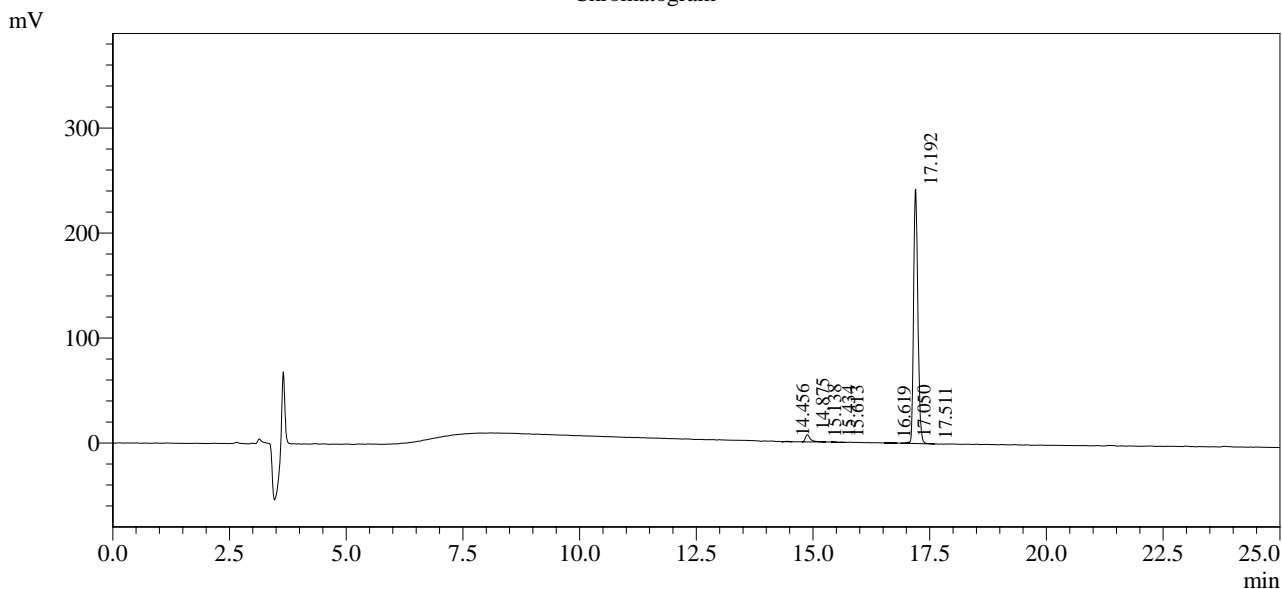

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.456	2867	414	0.177
2	14.875	51465	6787	3.174
3	15.138	1010	220	0.062
4	15.434	1439	221	0.089
5	15.613	1025	287	0.063
6	16.619	1588	206	0.098
7	17.050	4977	1131	0.307
8	17.192	1555876	242300	95.965
9	17.511	1042	236	0.064
Total		1621290	251802	100.000