

Sample Name :Peptide YY(PYY)(3-36),human  
 Cat No. : RP10354  
 Lot No. : PE8571902  
 Time Processed : 0:53:23  
 Month-Day-Year Processed : 02/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

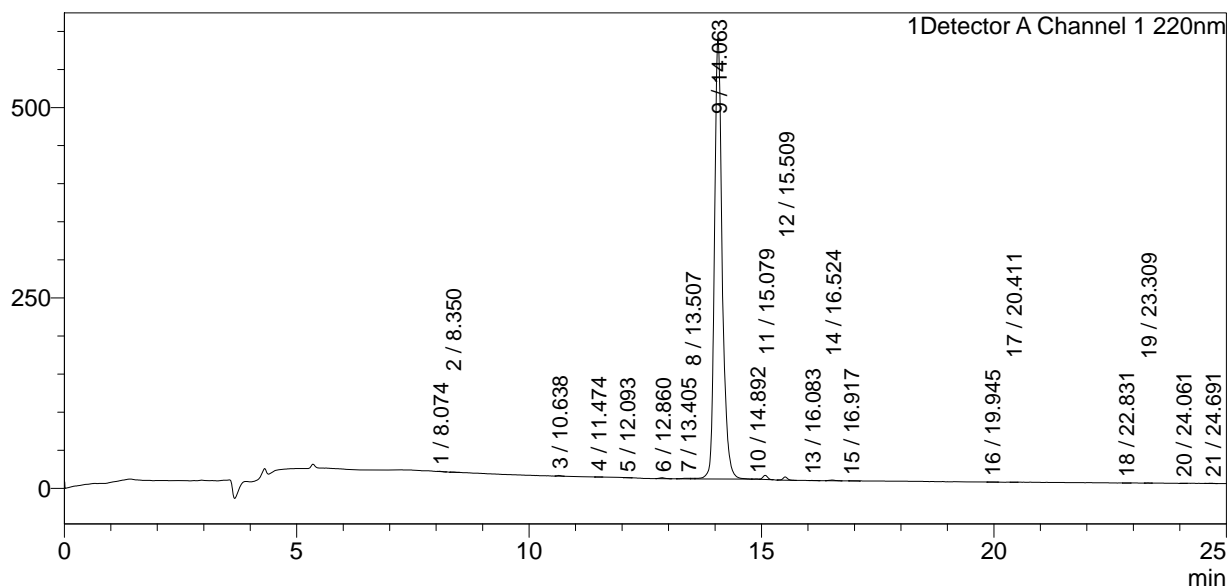

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.074	1378	320	0.020
2	8.350	1701	330	0.025
3	10.638	4192	800	0.061
4	11.474	1174	206	0.017
5	12.093	1783	273	0.026
6	12.860	9782	1219	0.143
7	13.405	9305	824	0.136
8	13.507	4191	796	0.061
9	14.063	6727765	578316	98.248
10	14.892	1662	270	0.024
11	15.079	36877	5360	0.539
12	15.509	28946	4293	0.423
13	16.083	1159	195	0.017
14	16.524	7915	916	0.116
15	16.917	1325	147	0.019

Peak#	Ret. Time	Area	Height	Area%
16	19.945	1068	134	0.016
17	20.411	1705	205	0.025
18	22.831	1425	183	0.021
19	23.309	1139	240	0.017
20	24.061	1002	163	0.015
21	24.691	2229	294	0.033
Total		6847723	595482	100.000