

Sample Name :EGFRvIII peptide (PEPvIII)
 Cat No.: RP20356
 Lot No.: E7957920B
 Time Processed :13:48:04
 Month-Day-Year Processed :02/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

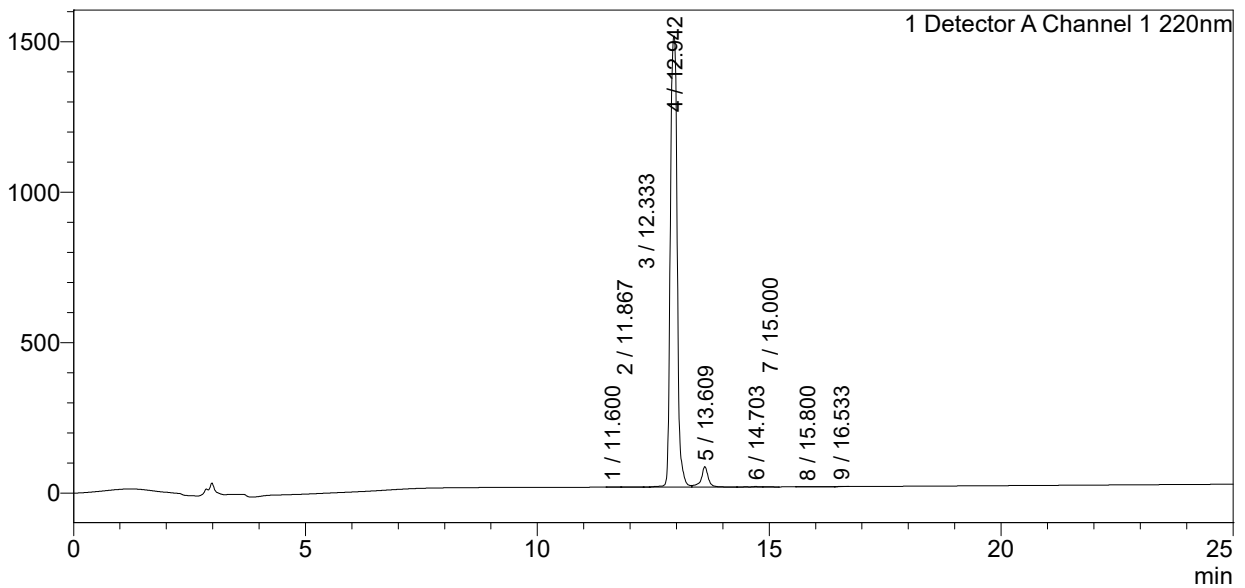

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.600	3939	365	0.025
2	11.867	6271	328	0.039
3	12.333	4183	548	0.026
4	12.942	15244586	1499083	95.271
5	13.609	712544	66359	4.453
6	14.703	16309	1459	0.102
7	15.000	7320	743	0.046
8	15.800	3829	208	0.024
9	16.533	2368	225	0.015
Total		16001349	1569319	100.000