

Sample Name :Endothelin 1, human, porcine
 Cat No. :RP12758
 Lot No. :PE5241901
 Time Processed :20:43:41
 Month-Day-Year Processed :01/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

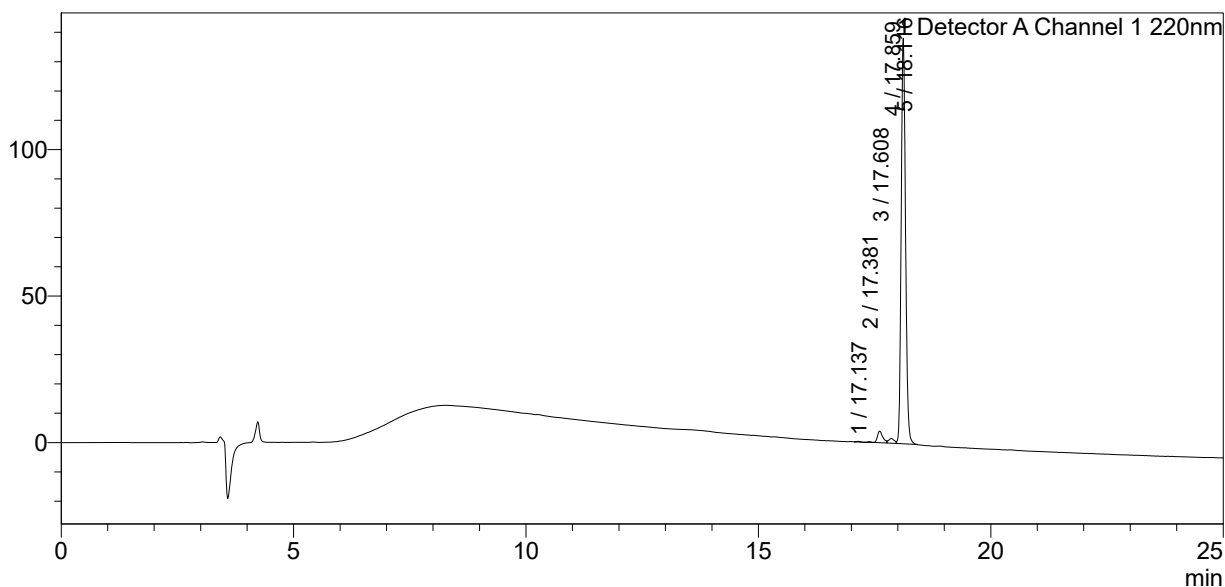

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.137	1299	205	0.137
2	17.381	1436	245	0.152
3	17.608	31017	3944	3.283
4	17.859	13463	1617	1.425
5	18.116	897525	138302	95.002
Total		944739	144313	100.000