

Sample Name: OVA G4 peptide
 Cat No: RP20398
 Lot NO: E7286920L
 Time Processed: 7:09:59
 Month-Day-Year Processed :12/24/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ17010509

<Chromatogram>

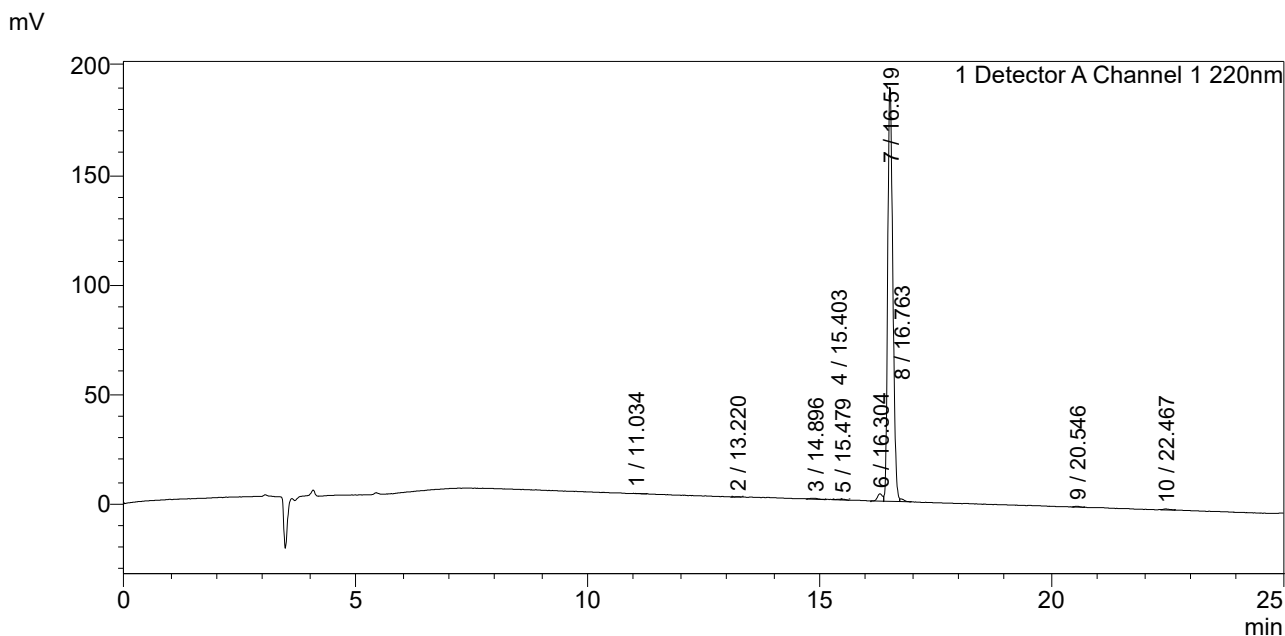

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.034	1075	144	0.072
2	13.220	1366	171	0.091
3	14.896	4673	428	0.311
4	15.403	1600	301	0.106
5	15.479	2730	341	0.182
6	16.304	25503	3390	1.697
7	16.519	1452130	188999	96.608
8	16.763	6310	1237	0.420
9	20.546	3202	428	0.213
10	22.467	4528	470	0.301
Total		1503116	195910	100.000