

Sample Name:OVA Peptide (323-339)
 Cat No :RP10610
 Lot No :E1940321E
 Time Processed :5:20:16 PM
 Month-Day-Year Processed :05/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

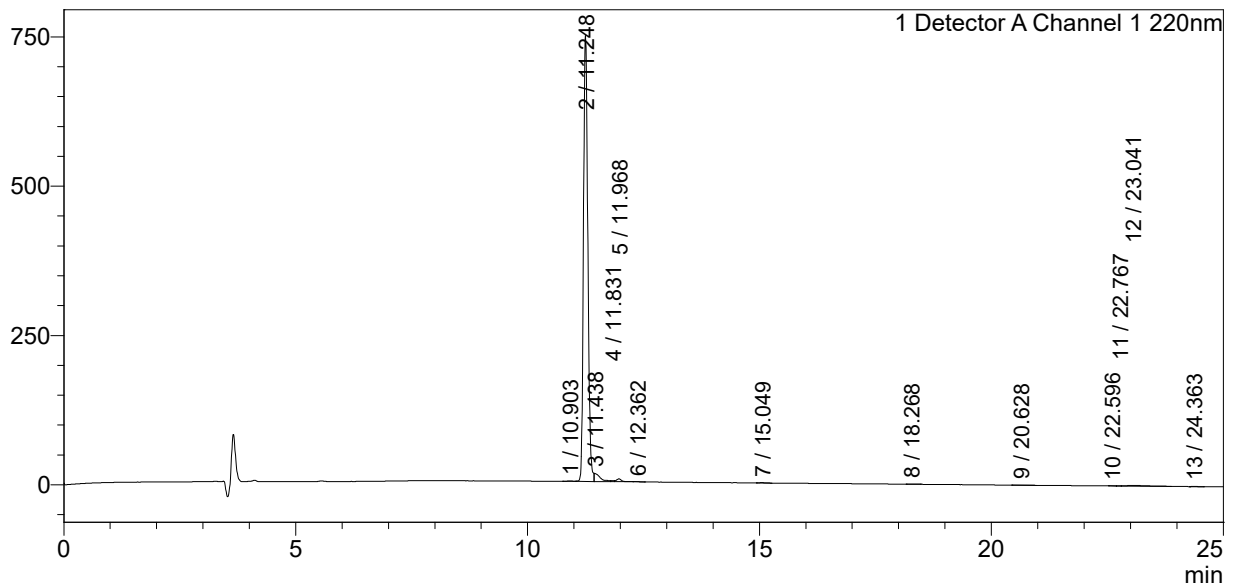

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.903	6347	572	0.124
2	11.248	4911048	746544	95.786
3	11.438	120151	13651	2.343
4	11.831	7837	1609	0.153
5	11.968	34288	4739	0.669
6	12.362	1866	287	0.036
7	15.049	3605	534	0.070
8	18.268	1727	264	0.034
9	20.628	3625	274	0.071
10	22.596	1228	151	0.024
11	22.767	1160	220	0.023
12	23.041	32468	1002	0.633
13	24.363	1758	176	0.034
Total		5127109	770022	100.000