

Sample Name :Gly-Arg-Gly-Asp-Asn-Pro
 Cat No :RP10847
 Lot No :E1278720J
 Time Processed :6:37:27
 Month-Day-Year Processed :10/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

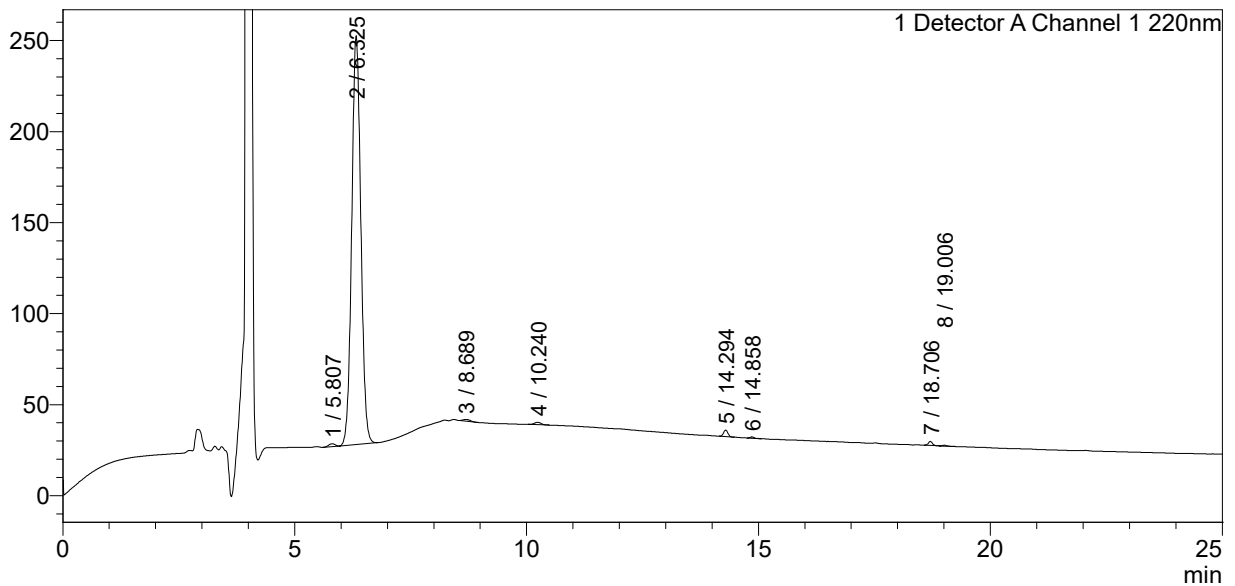

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.807	15903	1577	0.506
2	6.325	3058610	224705	97.279
3	8.689	10123	918	0.322
4	10.240	13964	1377	0.444
5	14.294	23771	3688	0.756
6	14.858	4420	764	0.141
7	18.706	14098	2252	0.448
8	19.006	3275	492	0.104
Total		3144163	235773	100.000