

Sample Name : Atrial Natriuretic Peptide (ANP) (1-28), rat
 Cat No.: RP11195
 Lot No.: E0972219K
 Time Processed : 20:58:44
 Month-Day-Year Processed : 12/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

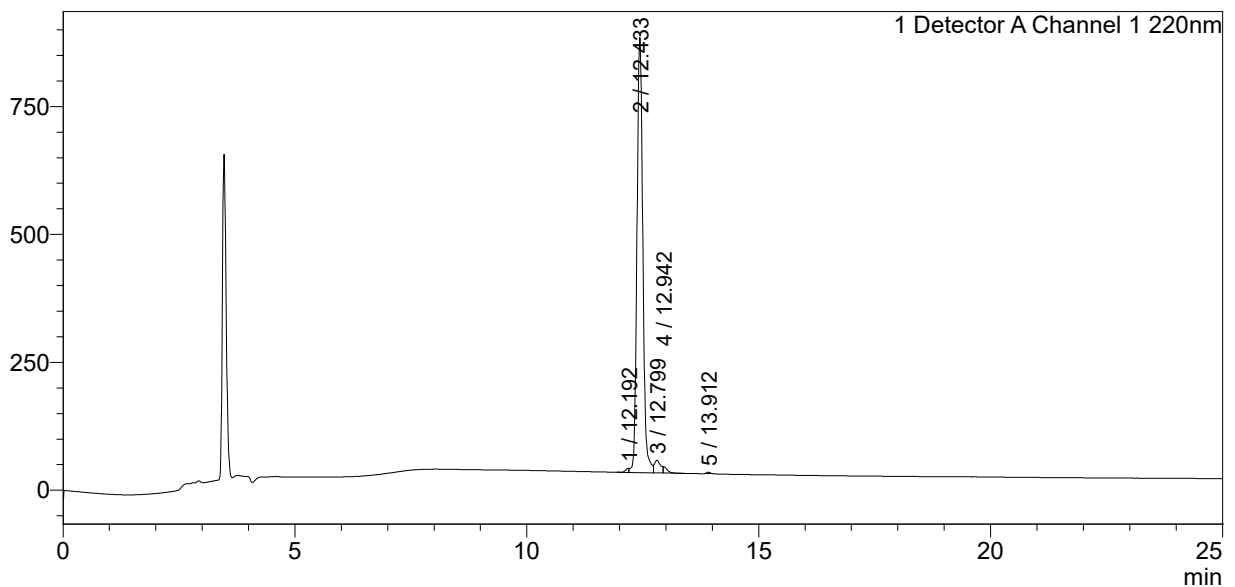

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.192	39678	8166	0.508
2	12.433	7460515	850790	95.524
3	12.799	229309	24841	2.936
4	12.942	69277	12214	0.887
5	13.912	11355	2342	0.145
Total		7810134	898352	100.000