

Sample Name :Prolactin Releasing Peptide (12-31), human  
 Cat No. :RP11864  
 Lot No. :E4877919I  
 Time Processed :3:30:35 AM  
 Month-Day-Year Processed :09/24/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

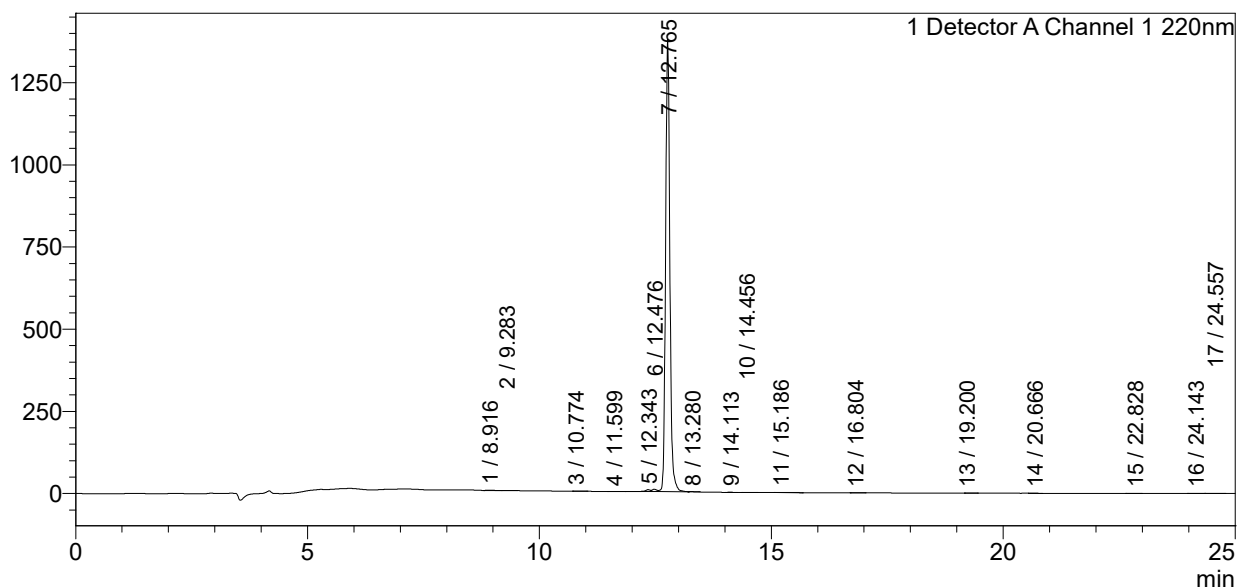

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.916	2817	206	0.031
2	9.283	3210	299	0.036
3	10.774	1127	106	0.013
4	11.599	1001	74	0.011
5	12.343	47854	5888	0.535
6	12.476	51058	7432	0.571
7	12.765	8820686	1377094	98.566
8	13.280	3500	616	0.039
9	14.113	2090	334	0.023
10	14.456	1176	133	0.013
11	15.186	3265	184	0.036
12	16.804	1134	116	0.013
13	19.200	1034	111	0.012
14	20.666	3924	552	0.044
15	22.828	1775	196	0.020

Peak#	Ret. Time	Area	Height	Area%
16	24.143	1462	108	0.016
17	24.557	1874	149	0.021
Total		8948987	1393597	100.000