

Sample Name :hgp100(25-33)  
 Cat No. :RP20344  
 Lot No. :E7831621E  
 Time Processed :16:05:20  
 Month-Day-Year Processed :05/08/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

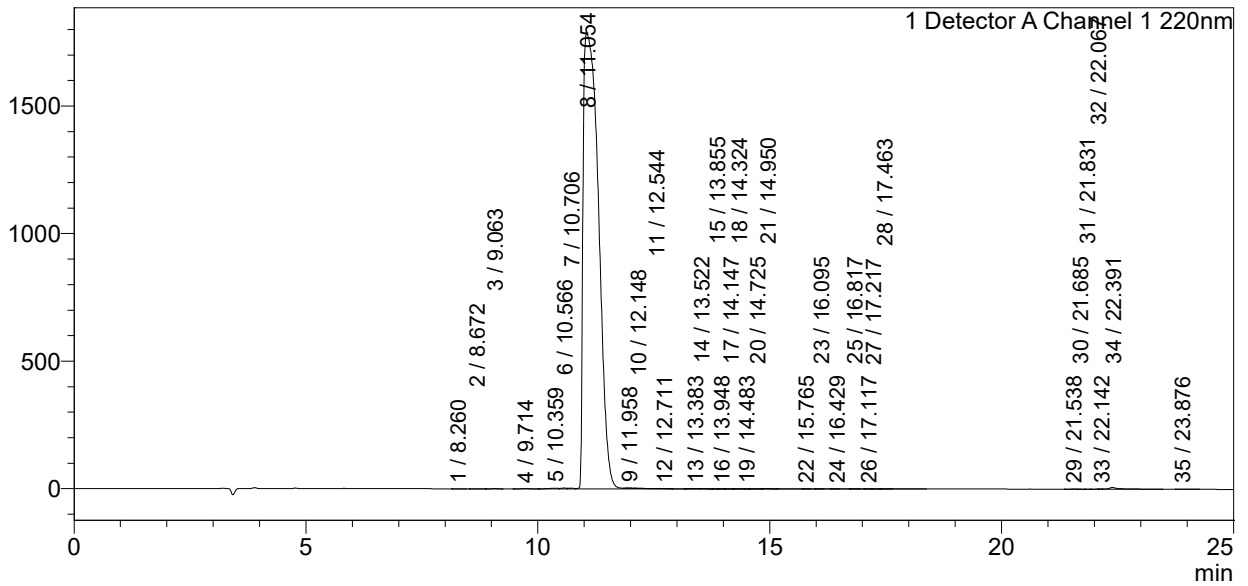

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.260	2092	305	0.005
2	8.672	3588	370	0.009
3	9.063	7872	856	0.019
4	9.714	18160	1381	0.044
5	10.359	40056	3038	0.096
6	10.566	31220	3423	0.075
7	10.706	27174	3238	0.065
8	11.054	41214860	1785090	99.219
9	11.958	9742	1023	0.023
10	12.148	8116	771	0.020
11	12.544	2080	295	0.005
12	12.711	7473	826	0.018
13	13.383	12990	1134	0.031
14	13.522	6985	815	0.017

Peak#	Ret. Time	Area	Height	Area%
15	13.855	1482	241	0.004
16	13.948	1918	256	0.005
17	14.147	2293	238	0.006
18	14.324	4311	344	0.010
19	14.483	1502	277	0.004
20	14.725	4585	365	0.011
21	14.950	9642	1103	0.023
22	15.765	1044	126	0.003
23	16.095	1900	200	0.005
24	16.429	1466	162	0.004
25	16.817	1095	98	0.003
26	17.117	1403	178	0.003
27	17.217	1461	165	0.004
28	17.463	2249	232	0.005
29	21.538	2792	270	0.007
30	21.685	2290	238	0.006
31	21.831	1467	220	0.004
32	22.067	2453	270	0.006
33	22.142	1250	286	0.003
34	22.391	97035	6620	0.234
35	23.876	3251	288	0.008
Total		41539296	1814742	100.000