

Sample Name :IRBP (1-20), human
 Cat. No. : RP20269
 Lot. No. : PE0191906
 Time Processed : 19:55:38
 Month-Day-Year Processed : 06/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
25.00	Pumps	Pump B Conc.	60	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

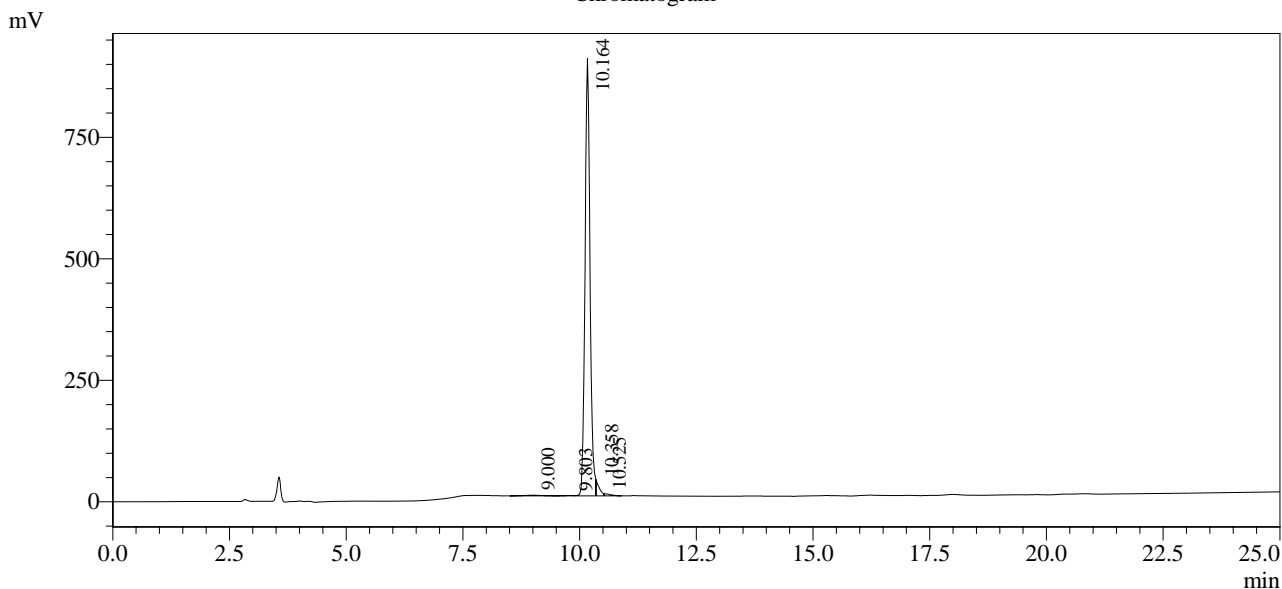

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.000	35298	1313	0.509
2	9.803	12586	862	0.181
3	10.164	6704812	900334	96.595
4	10.358	148824	30428	2.144
5	10.525	39607	4122	0.571
Total		6941128	937059	100.000