

Sample Name :β-amyloid (1-11)
 Cat No. :RP20106
 Lot No. :E2660520L
 Time Processed :8:06:45
 Month-Day-Year Processed :12/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

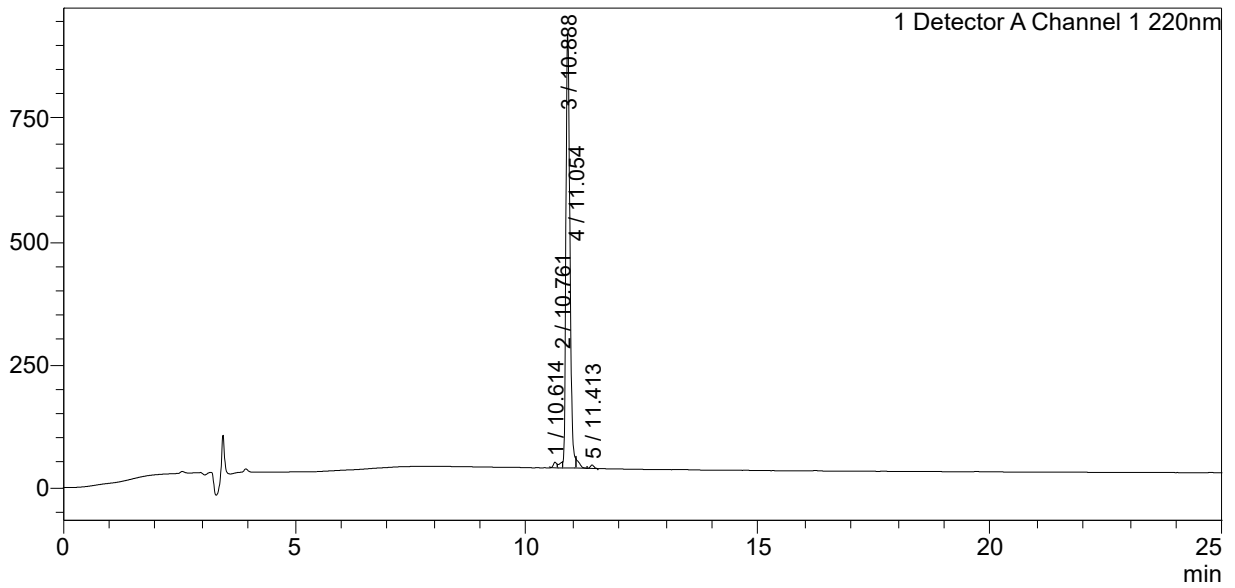

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.614	65802	11277	1.192
2	10.761	52388	11354	0.949
3	10.888	5249312	882634	95.089
4	11.054	116272	21656	2.106
5	11.413	36640	7001	0.664
Total		5520412	933921	100.000