

Sample Name :Rhodopsin Epitope Tag
 Cat No. : RP20400
 Lot No. : PE8861902
 Time Processed : 22:21:57
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

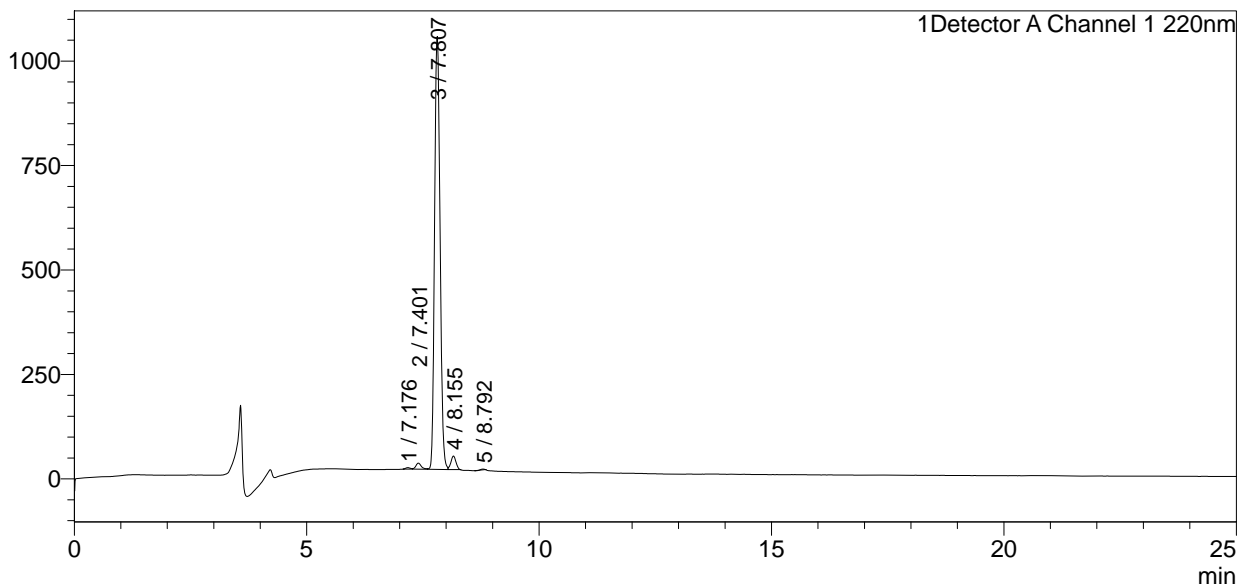

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.176	25848	3592	0.291
2	7.401	120684	14635	1.358
3	7.807	8487894	1036260	95.523
4	8.155	241876	32355	2.722
5	8.792	9390	1973	0.106
Total		8885692	1088815	100.000