

Sample Name :GnRH-I  
 Cat No. :RP20303  
 Lot No. :E2096120F  
 Time Processed :9:34:18 AM  
 Month-Day-Year Processed :06/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : AlltimaTM C18 4.6 x 250 mm  
 Equipment:ZJ19010141

<Chromatogram>

mV

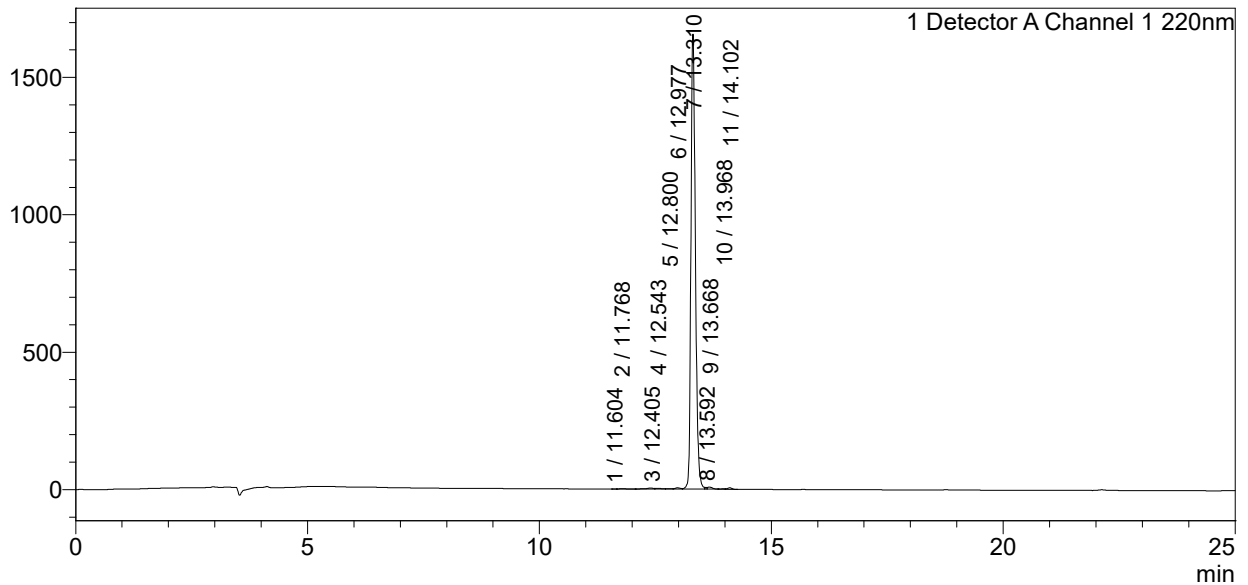

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.604	204	42	0.002
2	11.768	6340	586	0.056
3	12.405	37704	3195	0.331
4	12.543	22697	2319	0.199
5	12.800	12776	1653	0.112
6	12.977	33863	4482	0.297
7	13.310	11169538	1656143	98.032
8	13.592	19506	6536	0.171
9	13.668	48305	6802	0.424
10	13.968	8724	1505	0.077
11	14.102	34125	5232	0.300
Total		11393783	1688494	100.000