

Sample Name : Myomodulin
 Cat. No. : RP10606
 Lot. No. : E5716619F
 Time Processed : 10:24:55
 Month-Day-Year Processed : 06/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

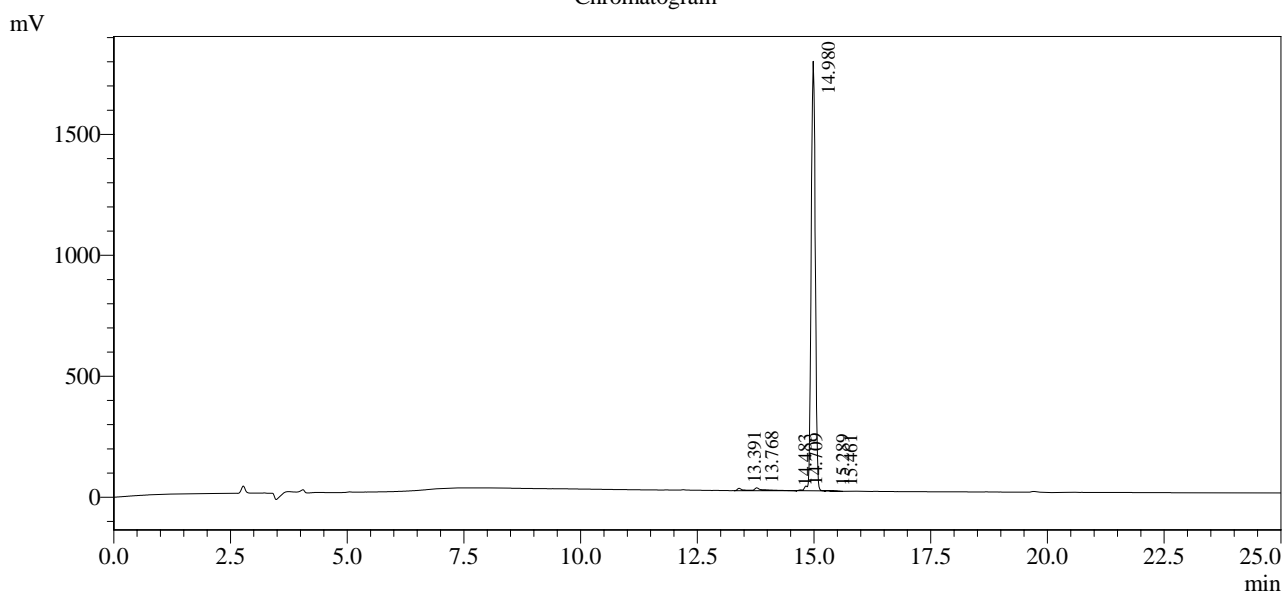

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.391	76020	9684	0.677
2	13.768	147032	11649	1.309
3	14.483	1009	188	0.009
4	14.709	15904	3261	0.142
5	14.980	10979760	1775699	97.764
6	15.289	7316	1671	0.065
7	15.461	3878	798	0.035
Total		11230919	1802950	100.000