

Sample Name:[Glu1]-Fibrinopeptide B
 Cat No: RP20439
 Lot No : E768921D
 Time Processed :12:56:50 PM
 Month-Day-Year Processed :04/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

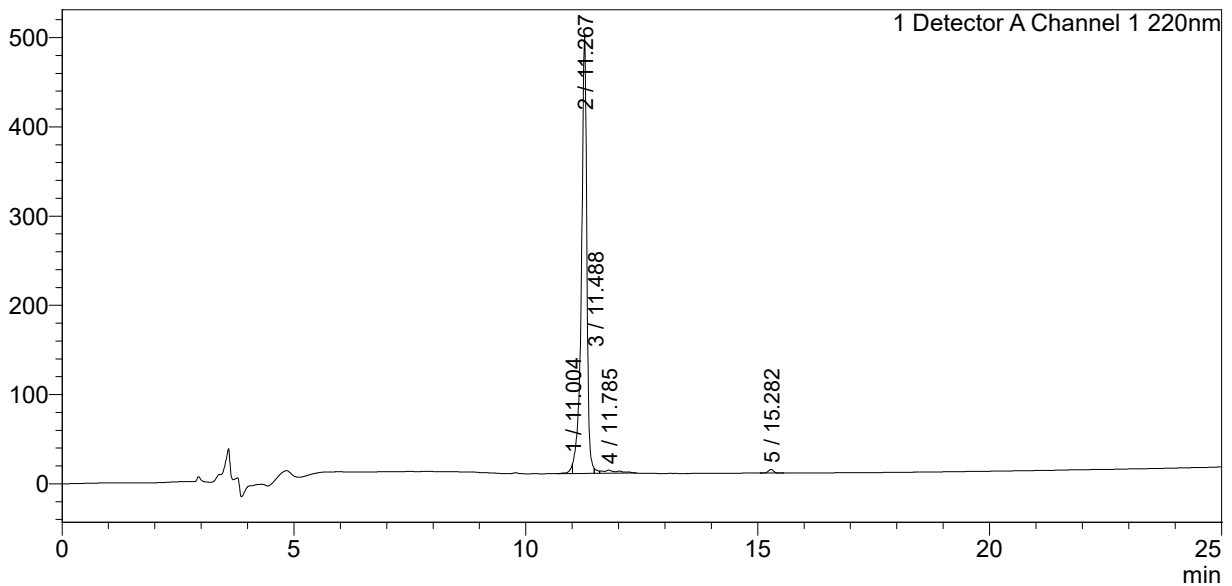

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.004	43019	9699	1.028
2	11.267	4006599	490769	95.764
3	11.488	23919	5054	0.572
4	11.785	80139	3446	1.915
5	15.282	30146	3951	0.721
Total		4183822	512919	100.000