

Sample Name : β -Amyloid (1-15)
 Cat No. :RP20141
 Lot No. :E0970019K
 Time Processed :8:32:30 AM
 Month-Day-Year Processed :11/24/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

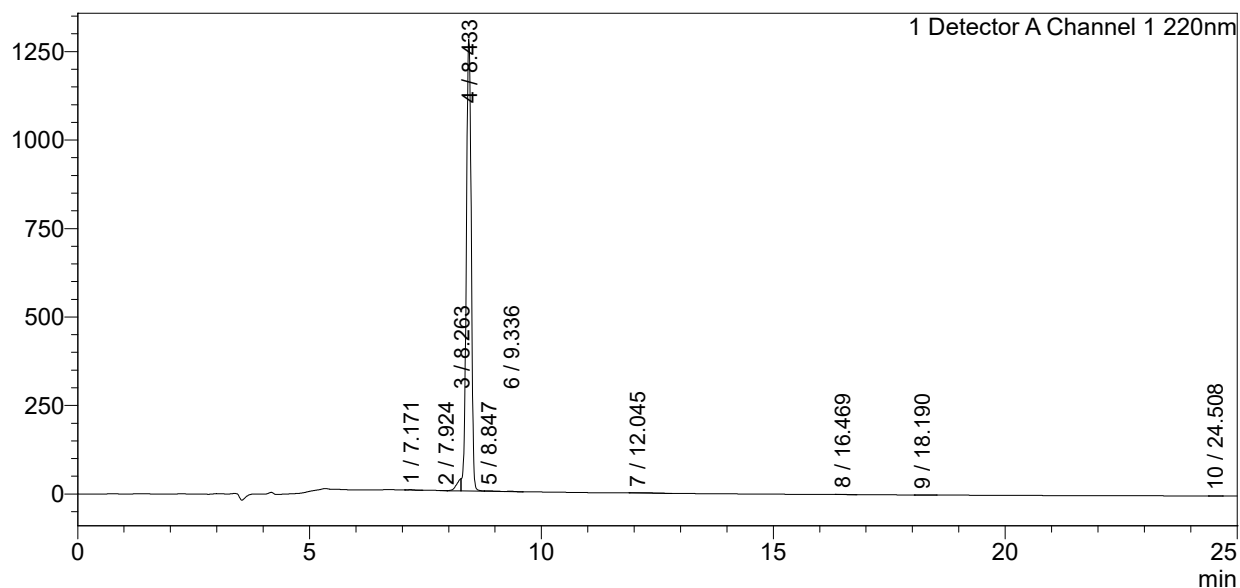

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.171	9244	1305	0.096
2	7.924	3592	582	0.037
3	8.263	230212	33878	2.379
4	8.433	9365145	1277172	96.788
5	8.847	22836	1395	0.236
6	9.336	15223	1405	0.157
7	12.045	19093	438	0.197
8	16.469	6077	673	0.063
9	18.190	3337	247	0.034
10	24.508	1134	110	0.012
Total		9675894	1317205	100.000