

Sample Name :Crustacean Cardioactive Peptide (CCAP)  
 Cat. No. : RP10572  
 Lot. No. : E6395020C  
 Time Processed :8:49:14  
 Month-Day-Year Processed : 03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

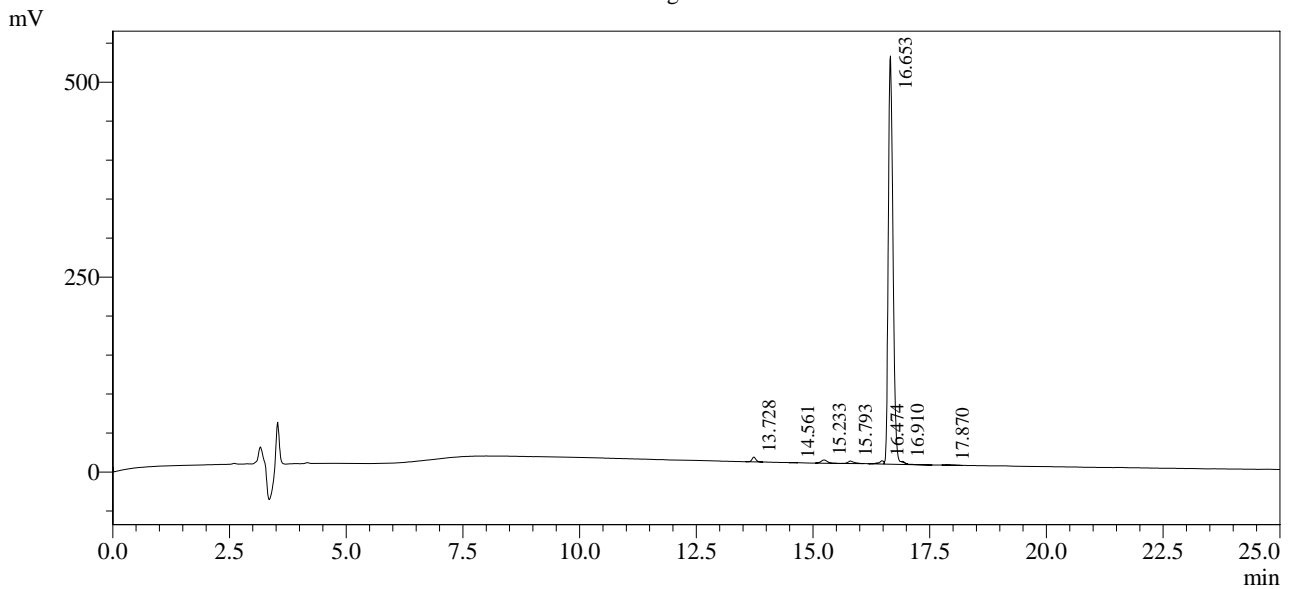

1 Det.A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.728	36006	6139	0.939
2	14.561	1189	208	0.031
3	15.233	41012	4170	1.069
4	15.793	29260	3109	0.763
5	16.474	29377	4092	0.766
6	16.653	3689995	523563	96.192
7	16.910	3783	917	0.099
8	17.870	5444	444	0.142
Total		3836066	542642	100.000