

Sample Name :Melanotan (MT)-II
 Cat No.: RP17323
 Lot No.: E0098419L
 Time Processed :13:21:53
 Month-Day-Year Processed :12/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

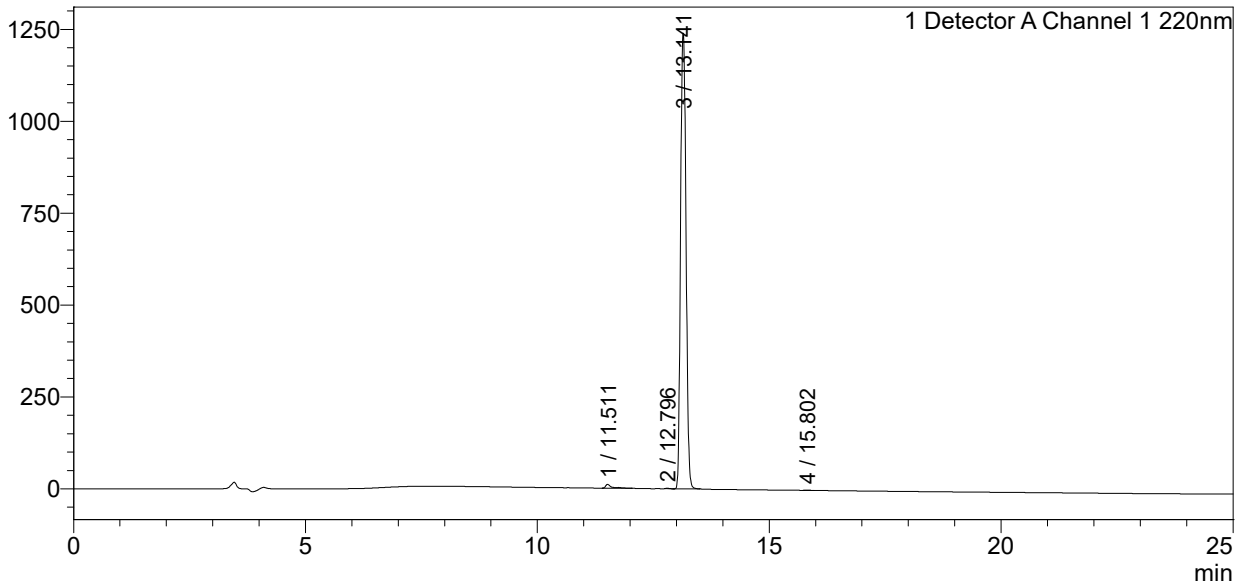

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.511	100073	10629	0.984
2	12.796	5799	1154	0.057
3	13.141	10060481	1240412	98.898
4	15.802	6274	1005	0.062
Total		10172627	1253200	100.000