

Sample Name :VIP, human, ovine, porcine, rat
 Cat. No. : RP10085
 Lot. No. : E1461619H
 Time Processed : 7:23:45 AM
 Month-Day-Year Processed : 08/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

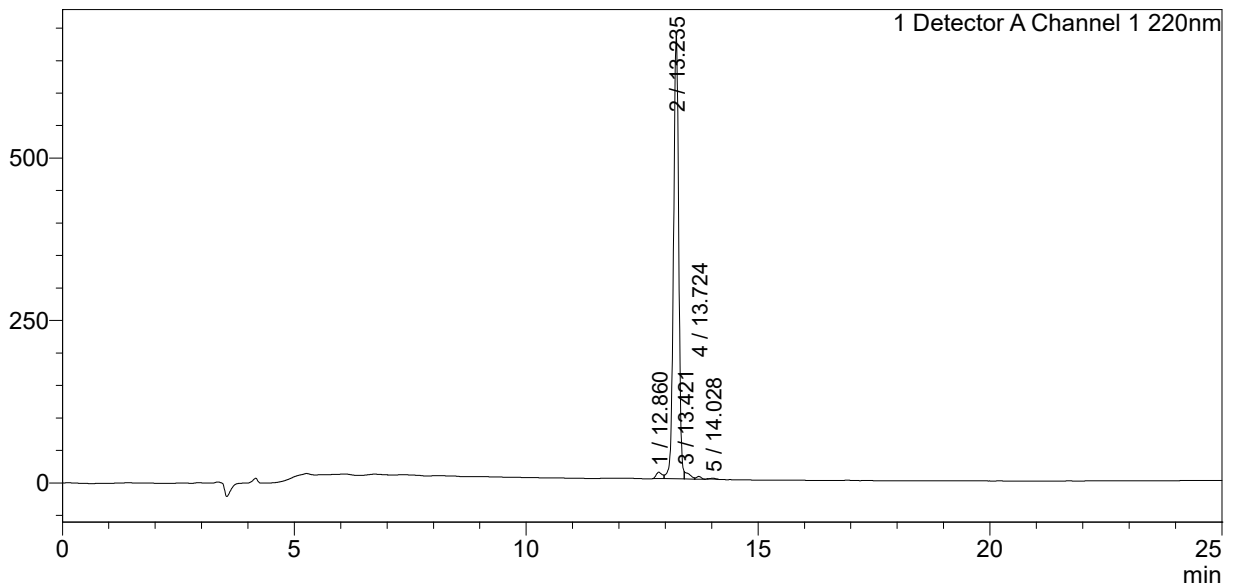

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.860	90627	9875	1.626
2	13.235	5359066	682589	96.154
3	13.421	84409	10463	1.514
4	13.724	28488	4135	0.511
5	14.028	10847	1586	0.195
Total		5573437	708647	100.000