

Sample Name : Octreotide (SMS 201-995)
 Cat. No. : RP10222
 Lot. No. : E47097191
 Time Processed : 8:46:14
 Month-Day-Year Processed : 10/12/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

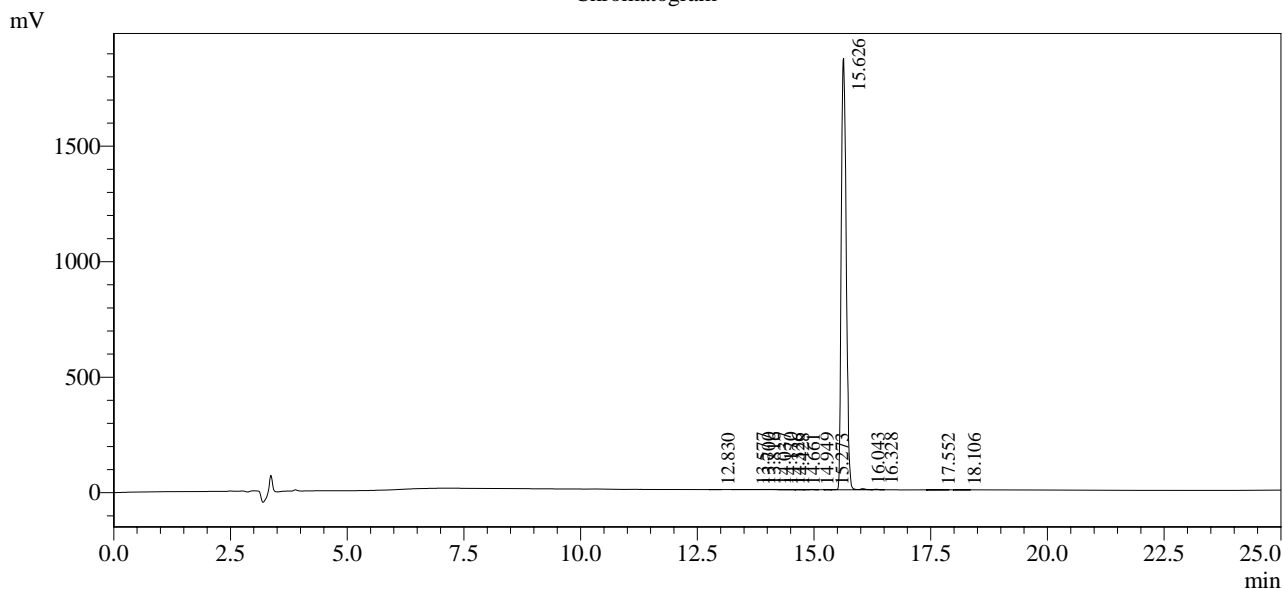

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.830	1294	192	0.009
2	13.577	13674	760	0.098
3	13.700	3440	692	0.025
4	13.816	9014	773	0.065
5	14.037	5710	792	0.041
6	14.170	8893	824	0.064
7	14.326	1604	385	0.011
8	14.428	2914	434	0.021
9	14.661	1070	206	0.008
10	14.949	8422	1157	0.060
11	15.273	1920	339	0.014
12	15.626	13840060	1868122	99.109
13	16.043	37416	4917	0.268
14	16.328	15930	2446	0.114
15	17.552	9567	919	0.069
16	18.106	3505	351	0.025
Total		13964433	1883308	100.000