

Sample Name : BDC2.5 mimotope 1040-31
 Cat. No. : RP20518
 Lot. No. : E5060720J
 Time Processed : 4:44:16 AM
 Month-Day-Year Processed : 10/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

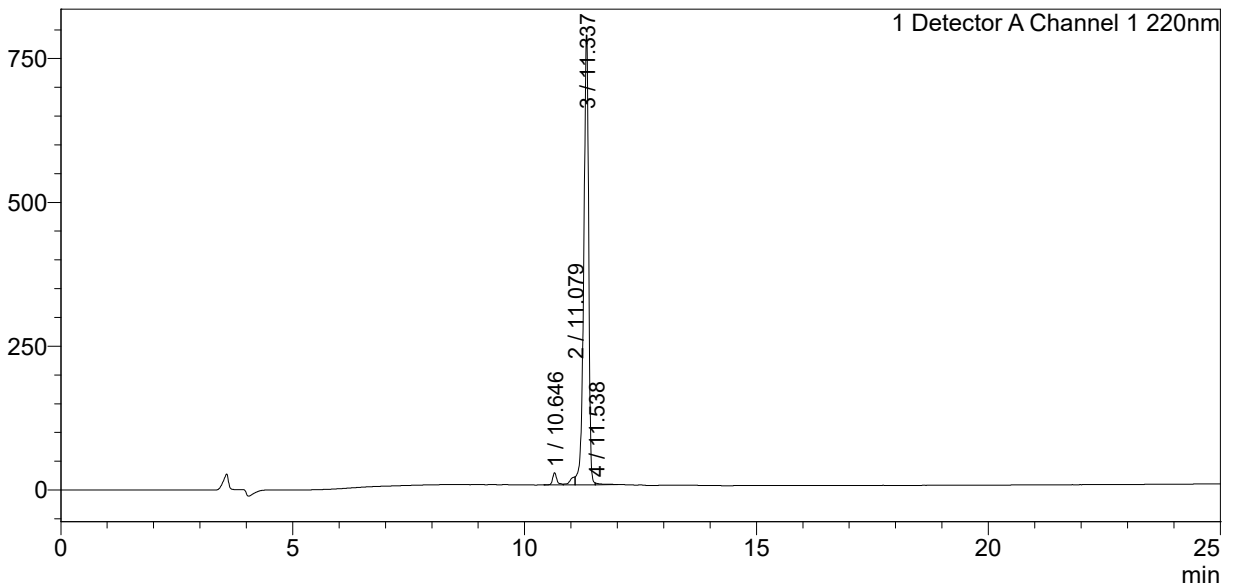

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.646	134553	21218	2.247
2	11.079	106083	13406	1.772
3	11.337	5720406	781947	95.543
4	11.538	26209	2799	0.438
Total		5987252	819370	100.000