

Sample Name : Gastrin-Releasing Peptide, human
 Cat. No. : RP10791
 Lot. No. : E9575719L
 Time Processed :7:33:29
 Month-Day-Year Processed :01/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

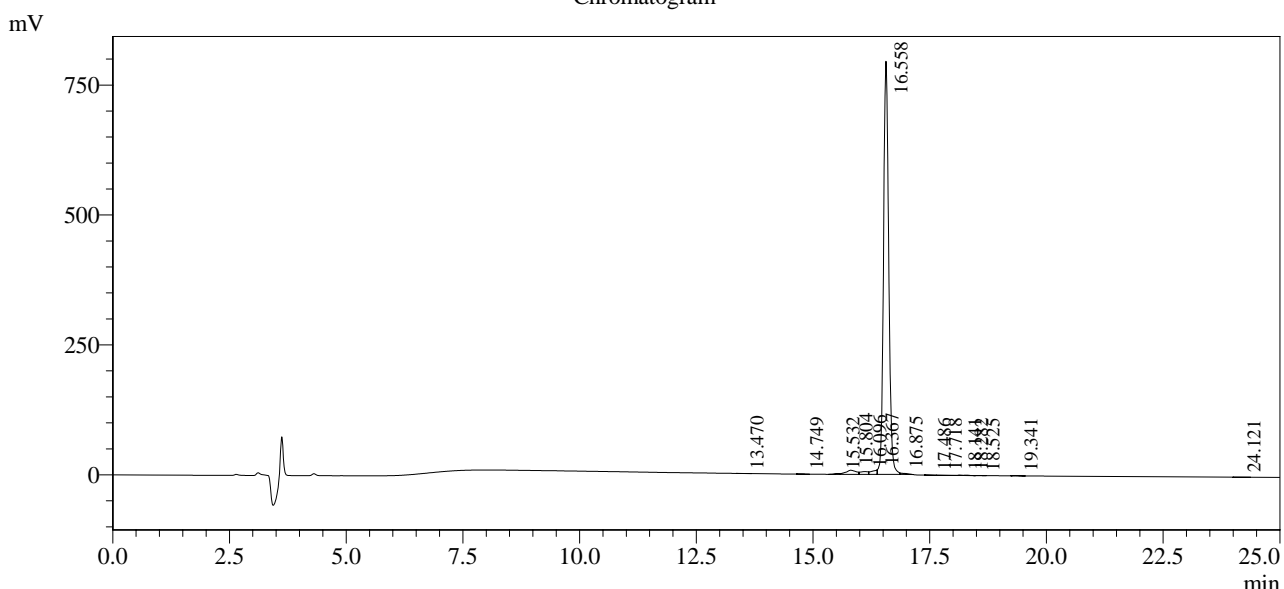

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.470	2263	235	0.035
2	14.749	1992	299	0.031
3	15.532	12811	1630	0.197
4	15.804	122579	7937	1.890
5	16.096	61527	5224	0.949
6	16.367	71742	8470	1.106
7	16.558	6166191	795039	95.058
8	16.875	23592	2680	0.364
9	17.486	2465	375	0.038
10	17.718	3515	554	0.054
11	18.141	5908	874	0.091
12	18.282	5370	816	0.083
13	18.525	1309	136	0.020
14	19.341	4049	544	0.062
15	24.121	1427	172	0.022
Total		6486739	824984	100.000