

Sample Name : Amylin, human, amide
 Cat. No. : RP11278
 Lot. No. : PE8751808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

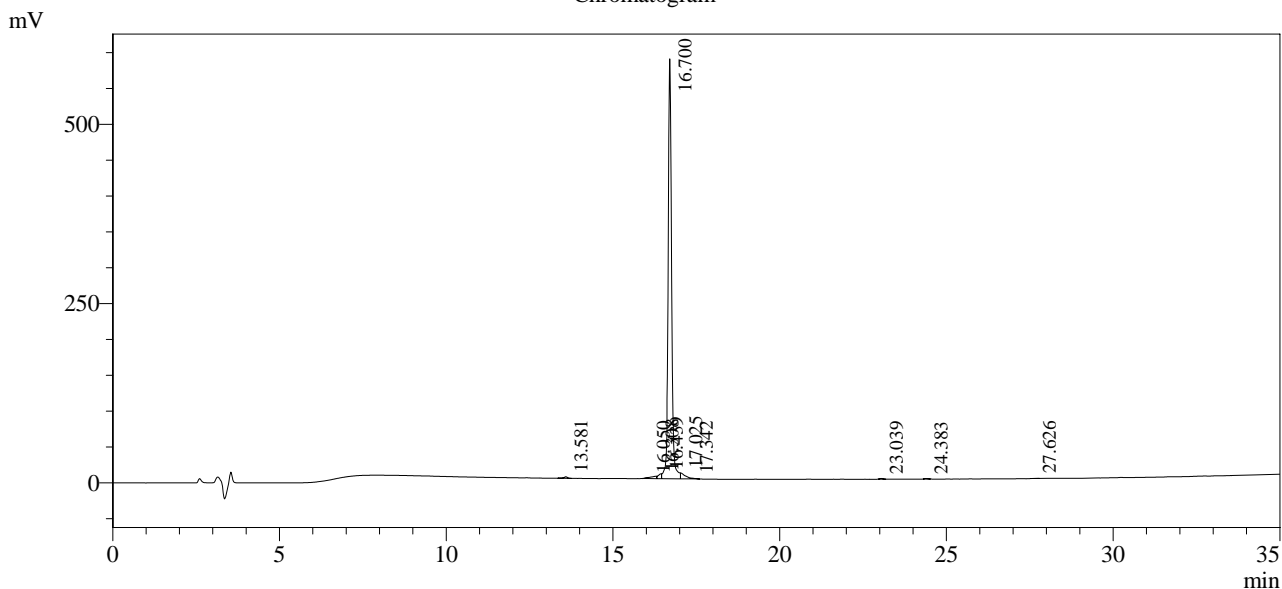

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.581	15542	2057	0.352
2	16.050	9892	1425	0.224
3	16.308	39285	3413	0.891
4	16.439	45735	6724	1.037
5	16.700	4199173	585621	95.210
6	17.025	78020	8243	1.769
7	17.342	8973	1163	0.203
8	23.039	5777	953	0.131
9	24.383	4117	606	0.093
10	27.626	3929	522	0.089
Total		4410443	610726	100.000