

Sample Name : Flagelin22  
 Cat. No. : RP19986  
 Lot. No. : E7119921A

Time Processed : 10:50:41  
 Month-Day-Year Processed : 01/16/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

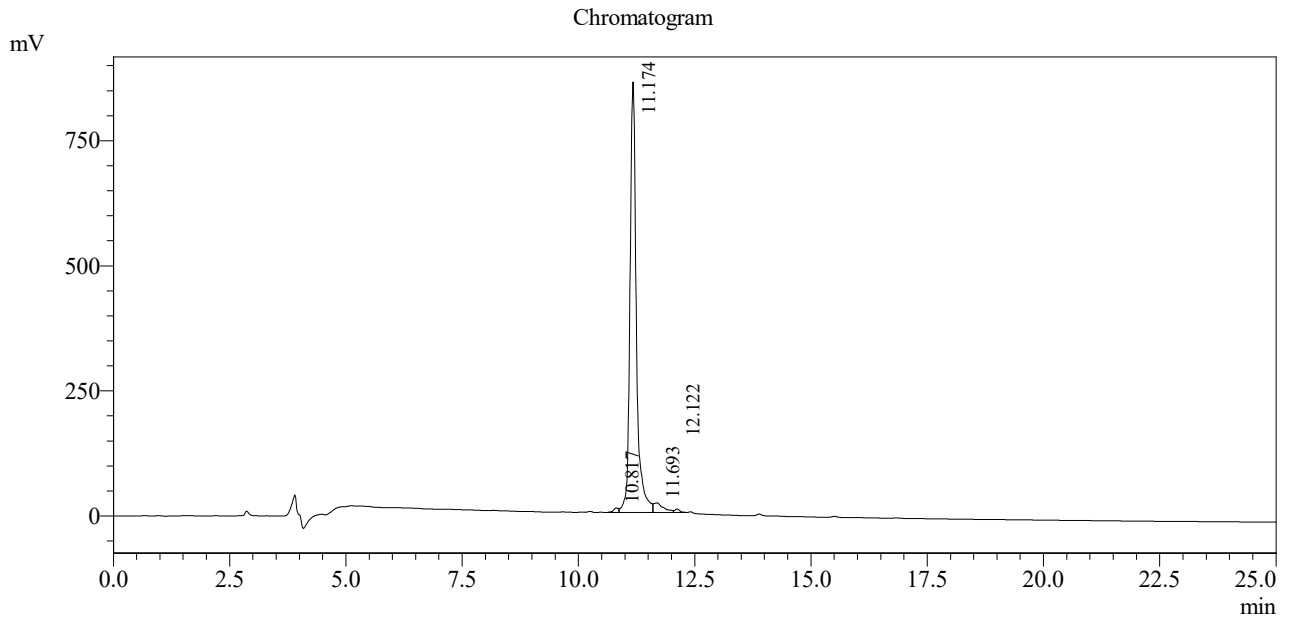

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.817	64864	8479	0.750
2	11.174	8261877	860341	95.483
3	11.693	278888	18651	3.223
4	12.122	47091	6953	0.544
Total		8652720	894423	100.000