

Sample Name : Pep-1 (uncapped)
 Cat. No. :RP10130
 Lot. No. :E4689019I
 Time Processed :13:02:21
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

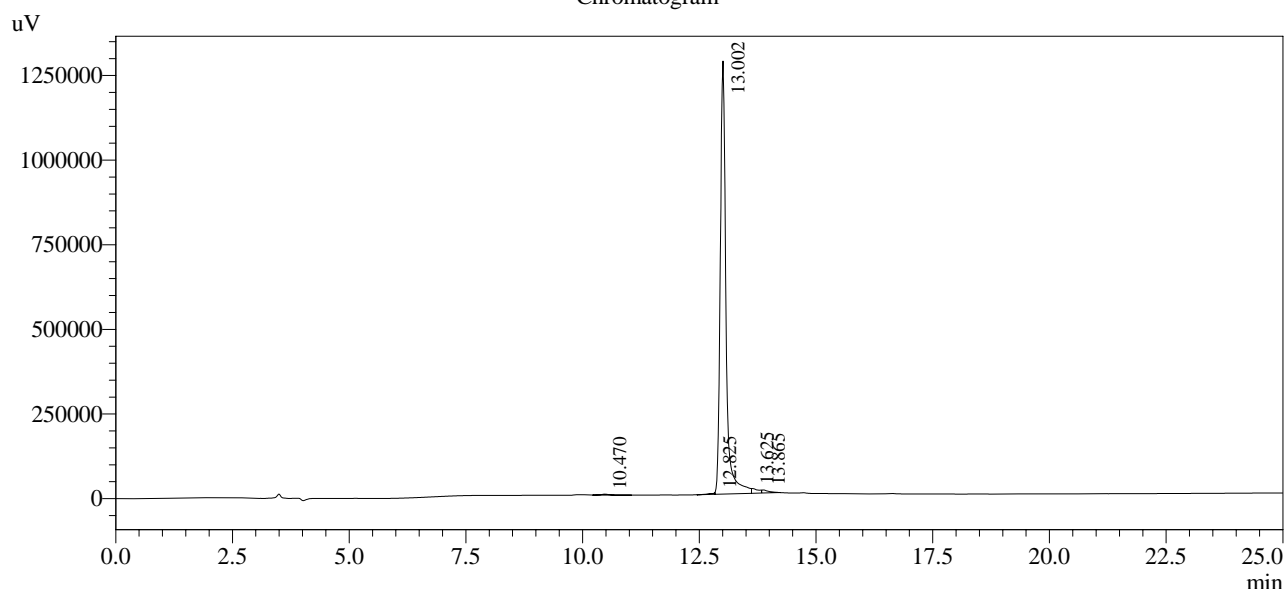

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.470	30298	2654	0.271
2	12.825	34137	4006	0.305
3	13.002	10902843	1279533	97.358
4	13.625	138949	14179	1.241
5	13.865	92465	9132	0.826
Total		11198693	1309503	100.000