

Sample Name : Somatostatin
 Cat. No. : RP10226
 Lot. No. : E3616419K
 Time Processed : 7:47:17
 Month-Day-Year Processed : 11/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

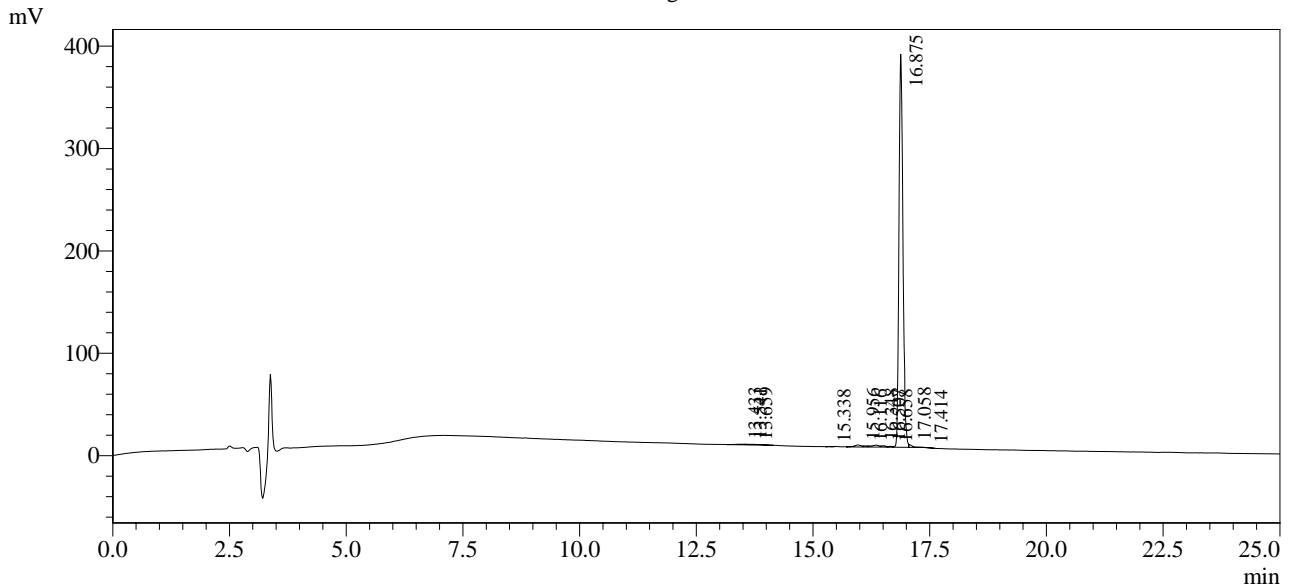

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.433	6817	603	0.286
2	13.541	5312	716	0.223
3	13.659	12482	686	0.524
4	15.338	1062	231	0.045
5	15.956	19808	1924	0.831
6	16.116	6531	1114	0.274
7	16.348	22731	1896	0.954
8	16.507	9377	1345	0.393
9	16.658	4791	751	0.201
10	16.875	2279006	383703	95.624
11	17.058	12638	2760	0.530
12	17.414	2752	364	0.115
Total		2383307	396091	100.000