

Sample Name :GnRH-I
 Cat. No. : RP20303
 Lot. No. : PE8761904
 Time Processed :8:49:38
 Month-Day-Year Processed : 04/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

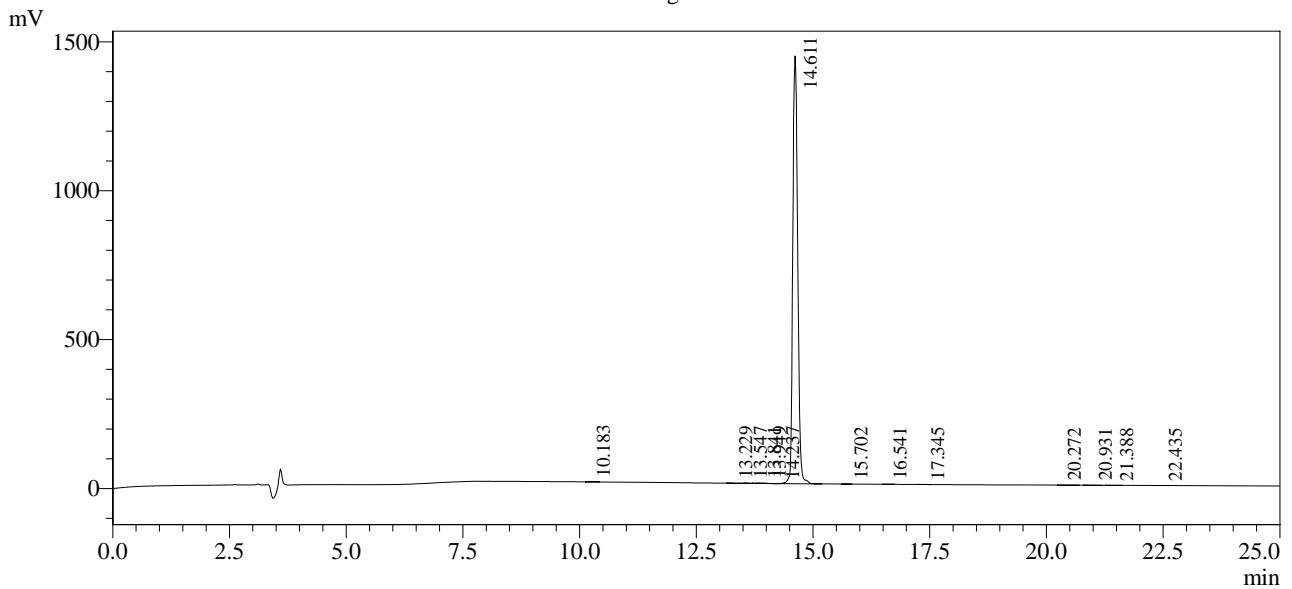

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.183	1268	155	0.012
2	13.229	3023	534	0.028
3	13.547	7492	1226	0.070
4	13.841	10360	1421	0.097
5	13.949	10321	1625	0.097
6	14.237	2930	529	0.028
7	14.611	10592328	1436376	99.521
8	15.702	1046	173	0.010
9	16.541	1592	226	0.015
10	17.345	1970	178	0.019
11	20.272	1014	48	0.010
12	20.931	4990	478	0.047
13	21.388	1470	127	0.014
14	22.435	3531	473	0.033
Total		10643337	1443568	100.000