


Mass Spectrum

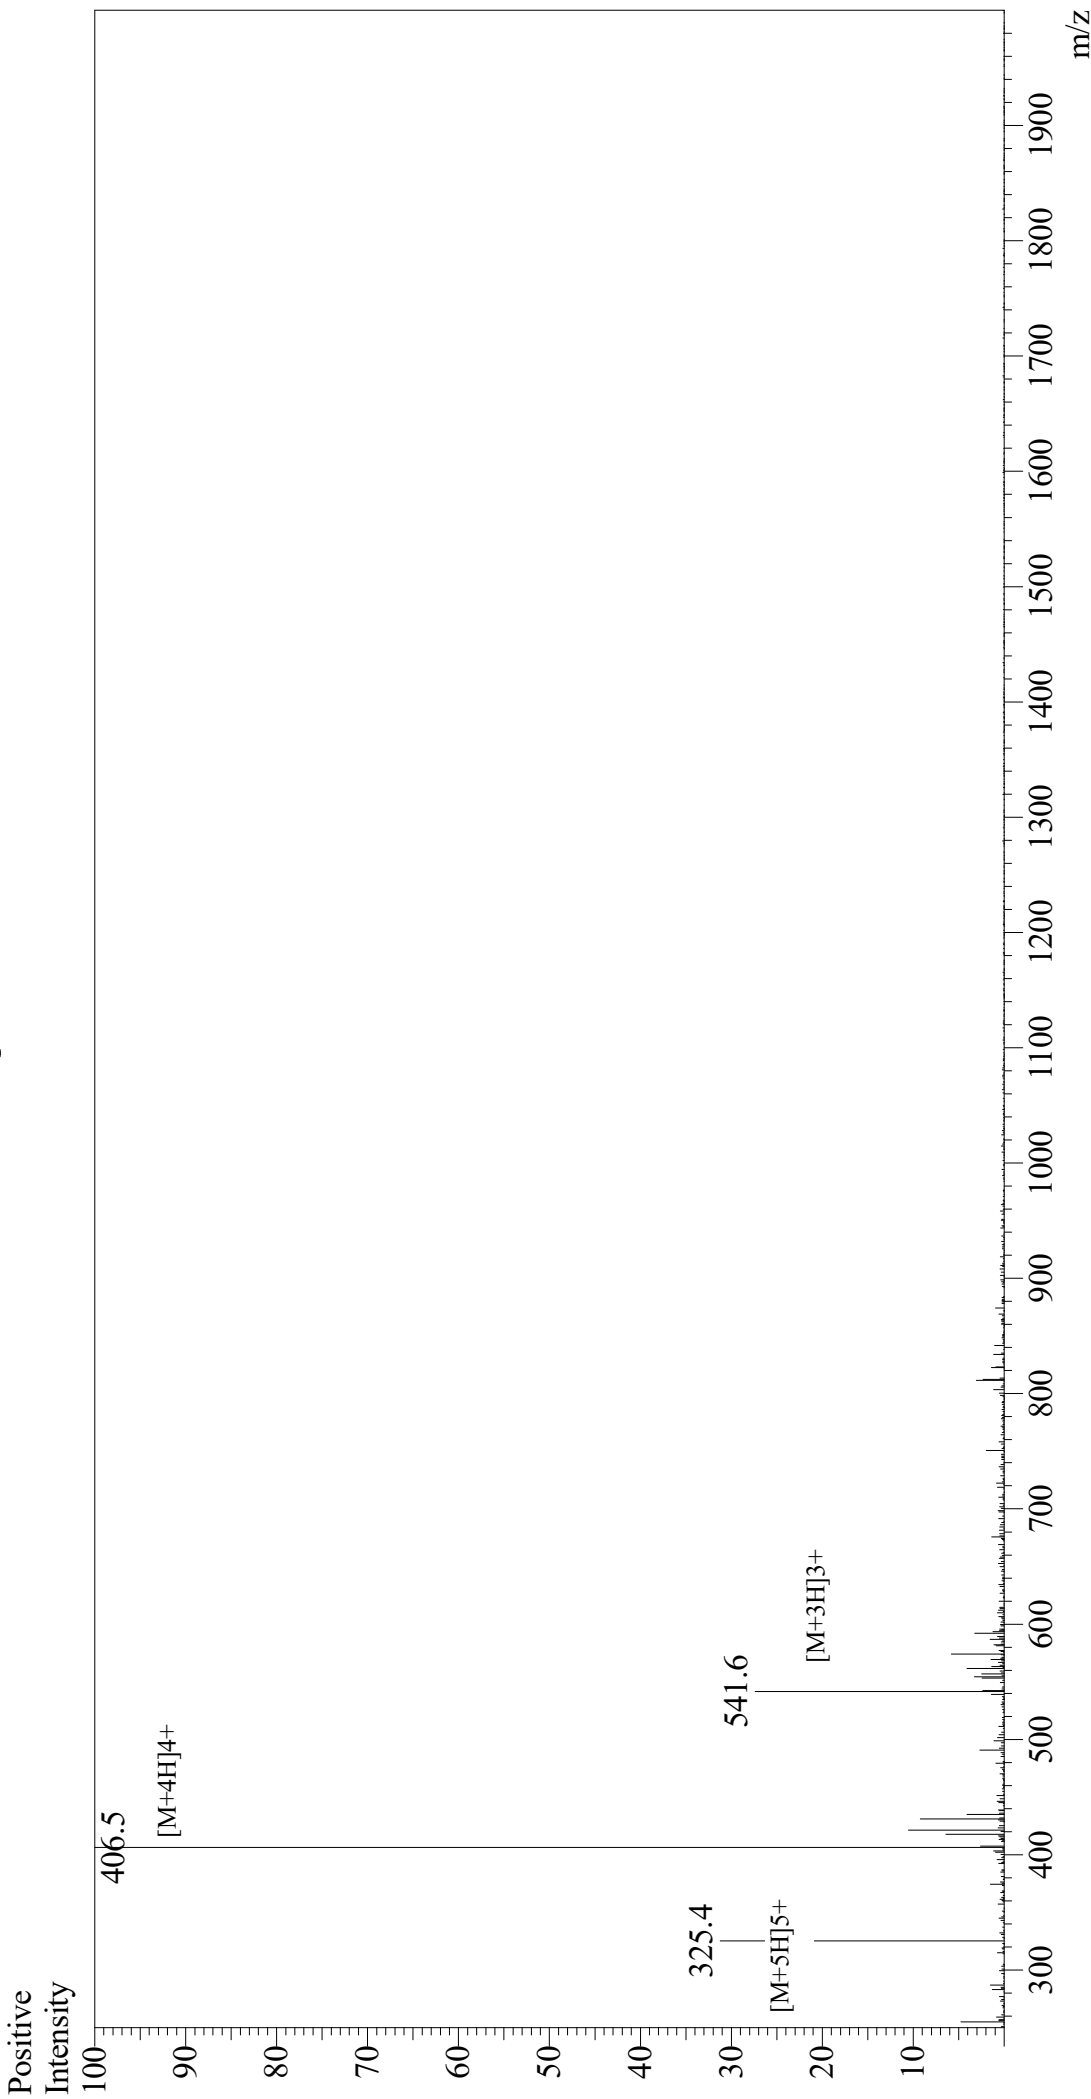

Sample Information

Month-Day Processed :	12/07/21	Equipment	: GK11010007
Time Processed :	13:13:35	Interface Bias	: +3.5 kV
Injection Volume :	0.2	Drying Gas Flow	: 5 L/min
Sample Name :	TAT peptide	T.Flow	: 0.2 ml/min
Cat No. :	RP20256	B.conc	: 50%H2O/50%MeOH
Lot No. :	E9979721K		
Theoretical MW :	1621.91		
Observed MW :	1622.0		