

Sample Name : $\beta$ -Amyloid (35-25)  
 Cat. No. : RP20185  
 Lot. No. : PE8801902  
 Time Processed : 14:06:42  
 Month-Day-Year Processed : 03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

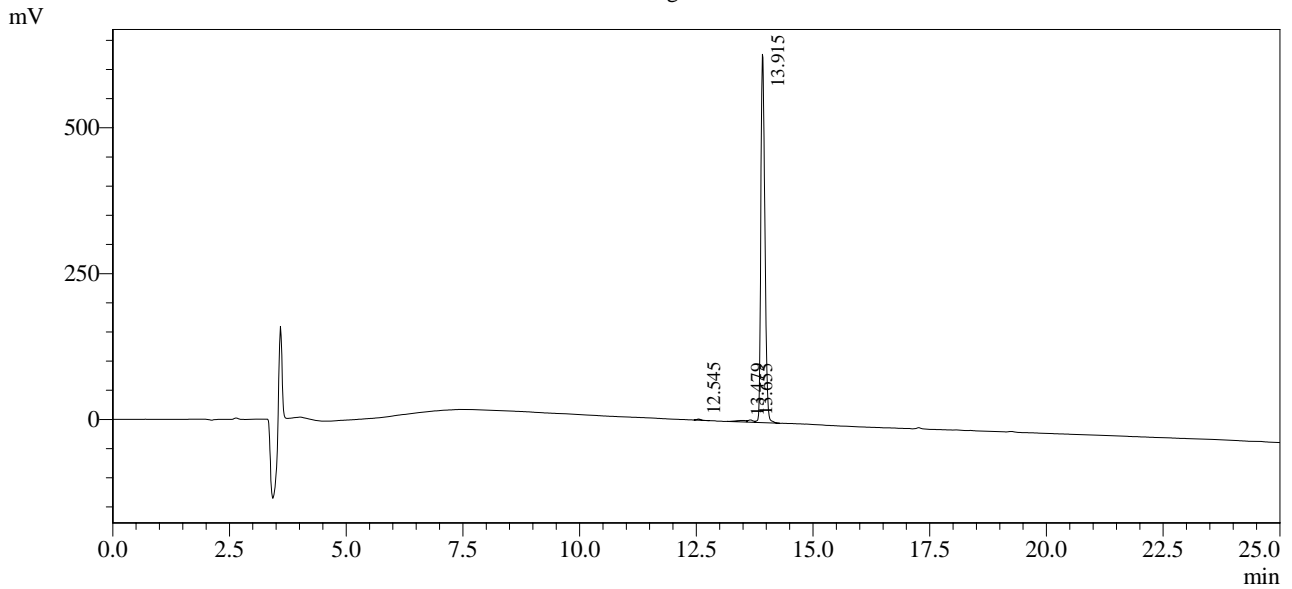

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.545	12256	1962	0.315
2	13.479	39170	2473	1.006
3	13.655	30968	3905	0.795
4	13.915	3812797	631643	97.885
Total		3895192	639983	100.000