

Sample Name :MOG (35-55)
 Cat No. :RP10245
 Lot No. :E4645519F
 Time Processed :9:06:26 PM
 Month-Day-Year Processed :06/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

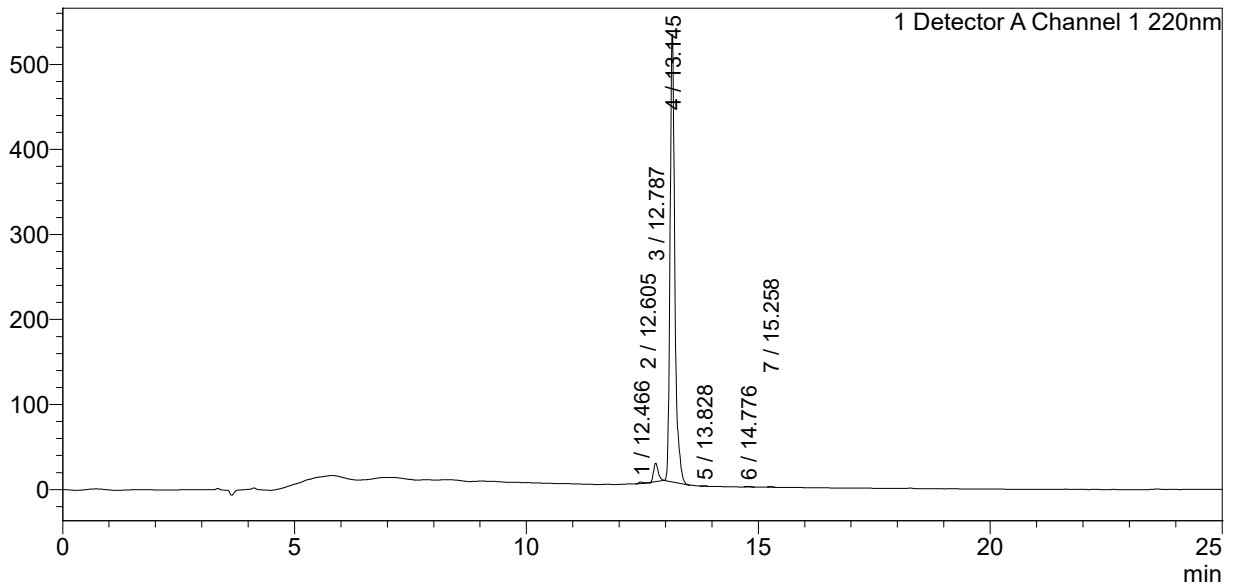

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.466	10880	1925	0.277
2	12.605	2812	632	0.072
3	12.787	152205	21698	3.872
4	13.145	3758150	526762	95.600
5	13.828	1639	404	0.042
6	14.776	2931	490	0.075
7	15.258	2507	575	0.064
Total		3931123	552485	100.000