

Sample Name : Neurotensin  
 Cat. No. : RP10439  
 Lot. No. : E2939920E  
 Time Processed : 4:10:49  
 Month-Day-Year Processed : 05/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

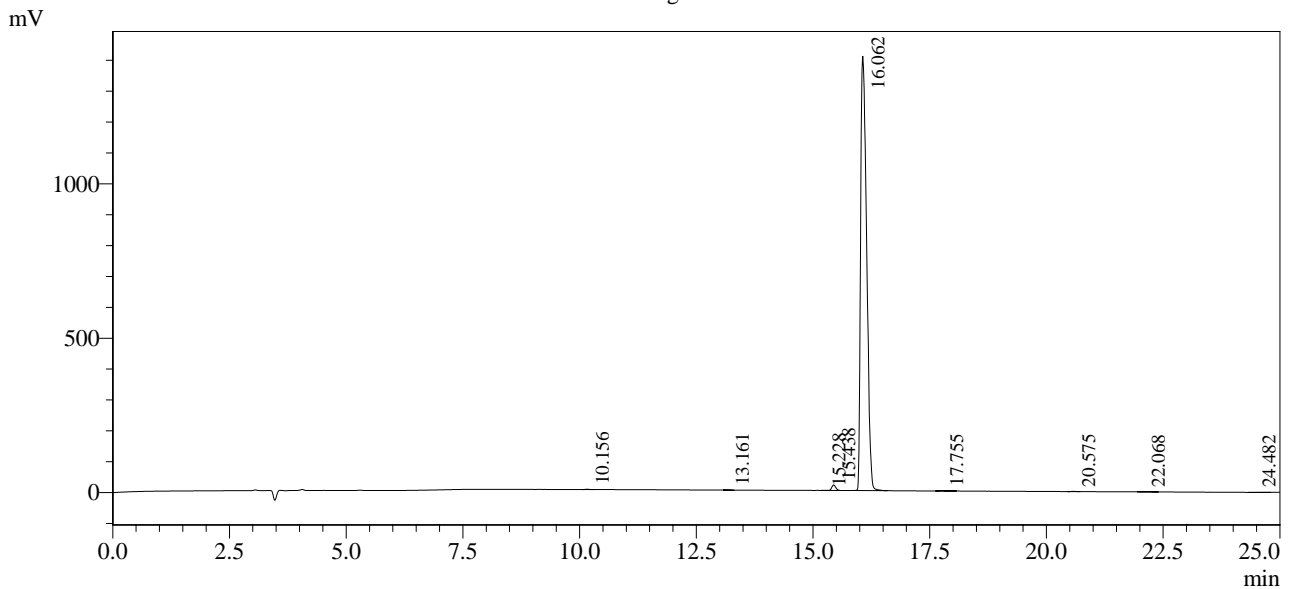

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.156	5091	1003	0.040
2	13.161	2355	396	0.018
3	15.228	2884	387	0.023
4	15.438	108072	18276	0.847
5	16.062	12625615	1406529	98.910
6	17.755	6515	881	0.051
7	20.575	4773	744	0.037
8	22.068	6114	479	0.048
9	24.482	3271	211	0.026
Total		12764690	1428905	100.000