

Sample Name :EGFRvIII peptide (PEPvIII)  
 Cat No. :RP20356  
 Lot No. :PE6321905  
 Time Processed :1:42:44 AM  
 Month-Day-Year Processed :05/29/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010141

<Chromatogram>

mV

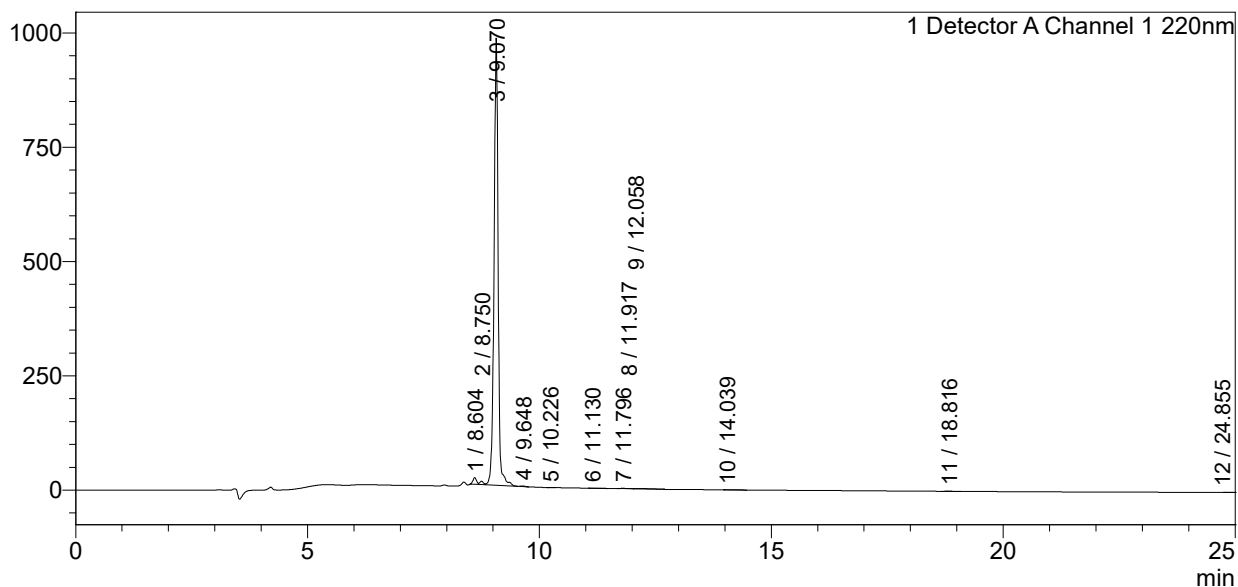

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.604	77115	14578	1.252
2	8.750	39256	7227	0.637
3	9.070	5994959	978201	97.306
4	9.648	4919	1040	0.080
5	10.226	1229	269	0.020
6	11.130	2912	260	0.047
7	11.796	4750	657	0.077
8	11.917	5852	626	0.095
9	12.058	22189	752	0.360
10	14.039	1670	75	0.027
11	18.816	4852	662	0.079
12	24.855	1204	128	0.020
Total		6160909	1004473	100.000