

Sample Name : Endothelin 1, human, porcine
 Cat No.: RP12758
 Lot No.: E0322719L
 Time Processed : 15:53:03
 Month-Day-Year Processed : 12/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
29.00	Pumps	Pump A B.Conc	95
29.01	Pumps	Pump A B.Conc	5
34.00	Pumps	Pump A B.Conc	5
60.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

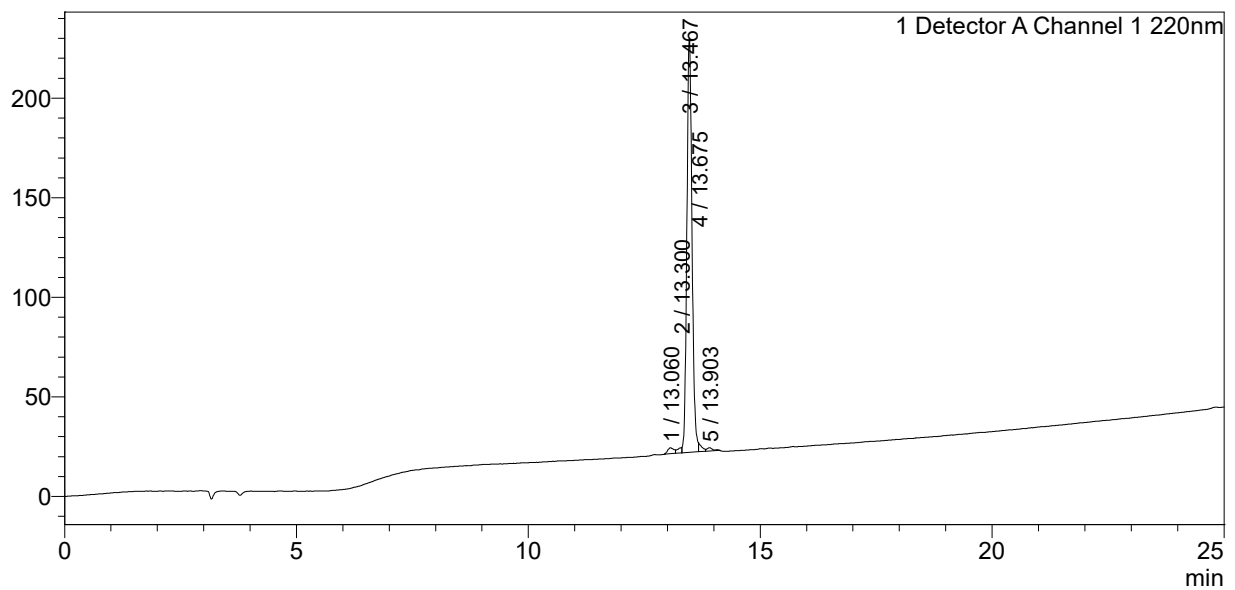

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.060	28100	2952	1.659
2	13.300	17752	2595	1.048
3	13.467	1611979	208140	95.191
4	13.675	21419	4151	1.265
5	13.903	14170	1659	0.837
Total		1693420	219496	100.000