

Sample Name :Heparin Binding Peptide
 Cat No. :RP13456
 Lot No. :E4913219I
 Time Processed :8:40:48 AM
 Month-Day-Year Processed :09/23/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

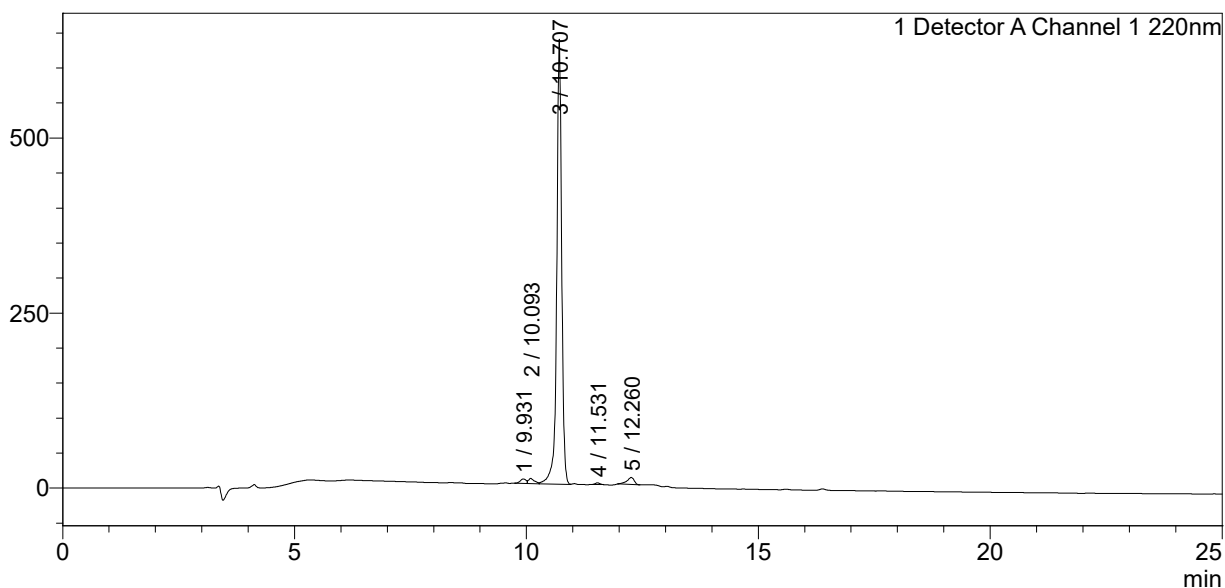

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.931	56354	6358	1.141
2	10.093	66692	7518	1.350
3	10.707	4692868	635799	95.026
4	11.531	15743	2426	0.319
5	12.260	106826	9891	2.163
Total		4938484	661991	100.000