

Sample Name :sgp91 ds-tat Peptide 2, scrambled  
 Cat No.: RP20436  
 Lot No.: E4976620B  
 Time Processed :17:04:31  
 Month-Day-Year Processed :02/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

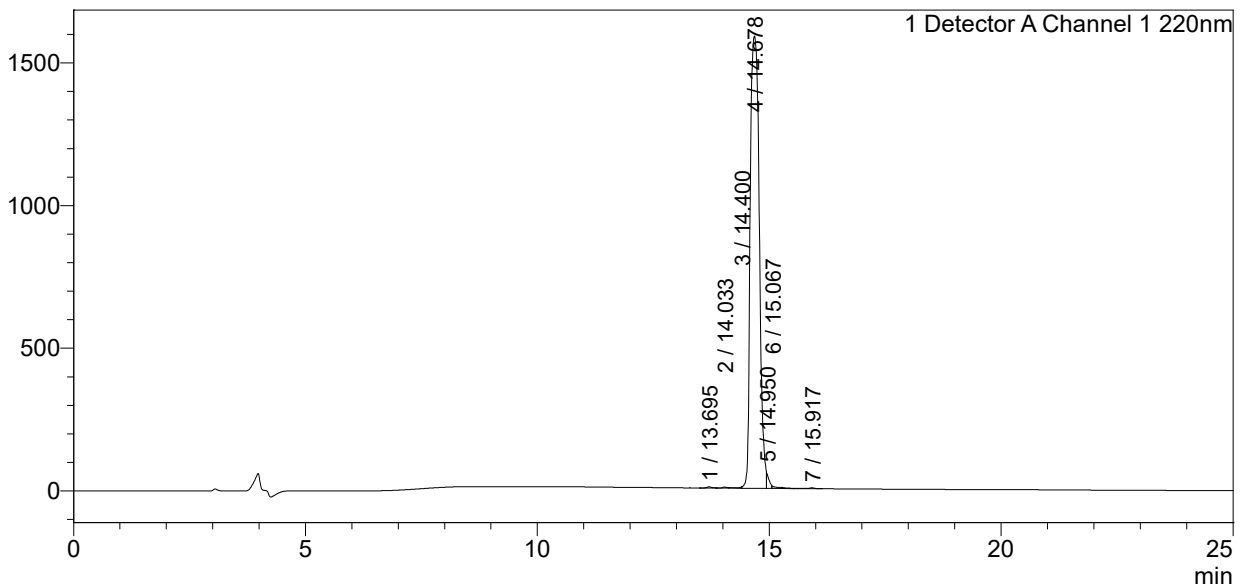

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.695	30933	4085	0.142
2	14.033	24272	3684	0.111
3	14.400	32961	4402	0.151
4	14.678	21431921	1585638	98.187
5	14.950	195461	52325	0.895
6	15.067	82083	8342	0.376
7	15.917	30046	2738	0.138
Total		21827675	1661215	100.000