

Sample Name :Bombesin

Cat No. :RP11157

Lot. No. :E5856119L

Time Processed :8:10:45

Month-Day-Year Processed :12/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

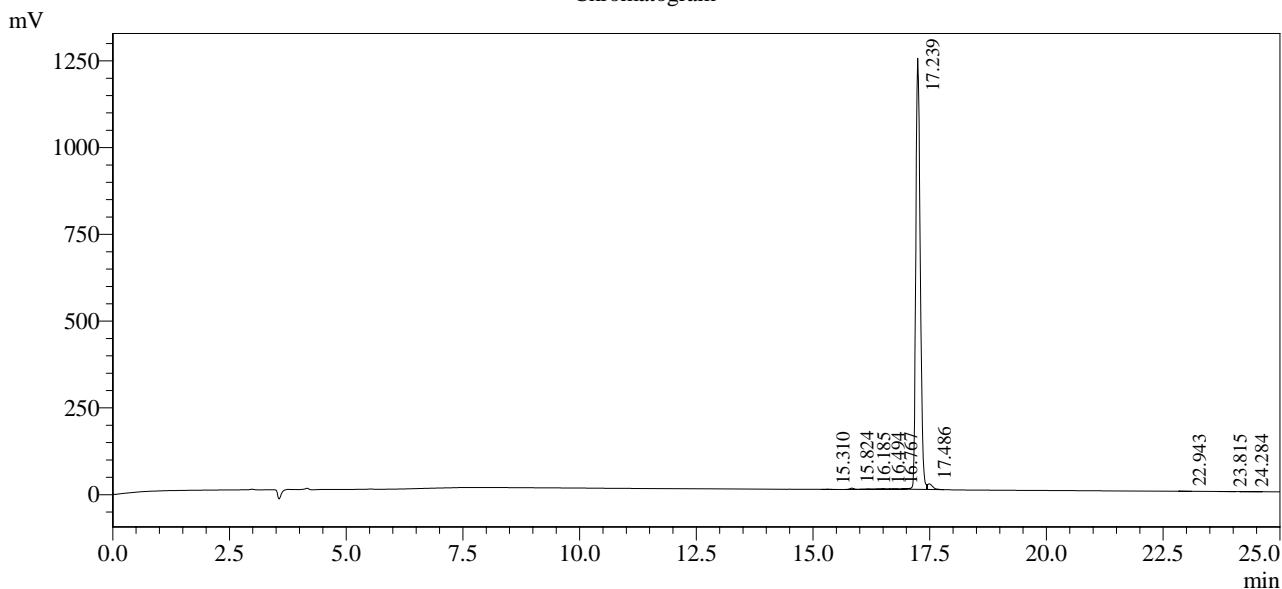

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.310	4148	586	0.049
2	15.824	23099	3682	0.273
3	16.185	13570	911	0.160
4	16.494	13993	1143	0.165
5	16.767	5232	601	0.062
6	17.239	8270112	1242124	97.635
7	17.486	124030	16028	1.464
8	22.943	3564	537	0.042
9	23.815	3325	429	0.039
10	24.284	9365	941	0.111
Total		8470437	1266982	100.000