

Sample Name :Rhodopsin Epitope Tag  
 Cat. No. : RP20400  
 Lot. No. :E4947119I  
 Time Processed :11:11:42  
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

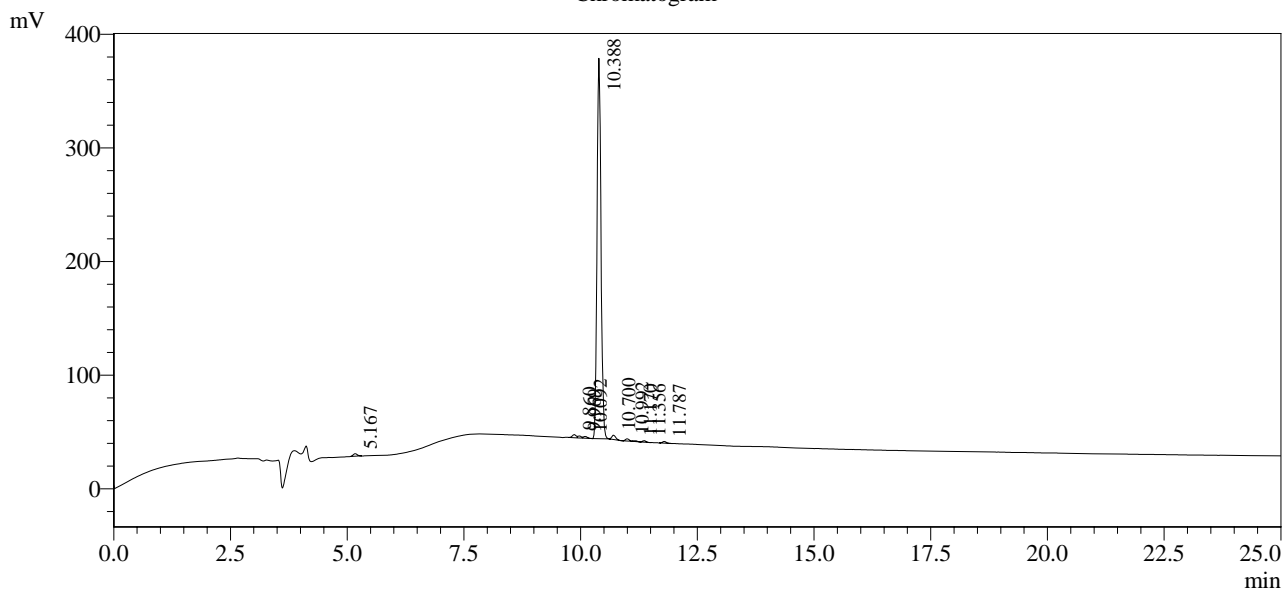

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.167	14021	2227	0.673
2	9.860	15933	2688	0.765
3	9.969	8534	1701	0.410
4	10.092	8956	1535	0.430
5	10.388	1983982	334877	95.239
6	10.700	22128	3817	1.062
7	10.992	10879	1920	0.522
8	11.170	3262	693	0.157
9	11.356	7352	1349	0.353
10	11.787	8111	1429	0.389
Total		2083158	352238	100.000