


Mass Spectrum

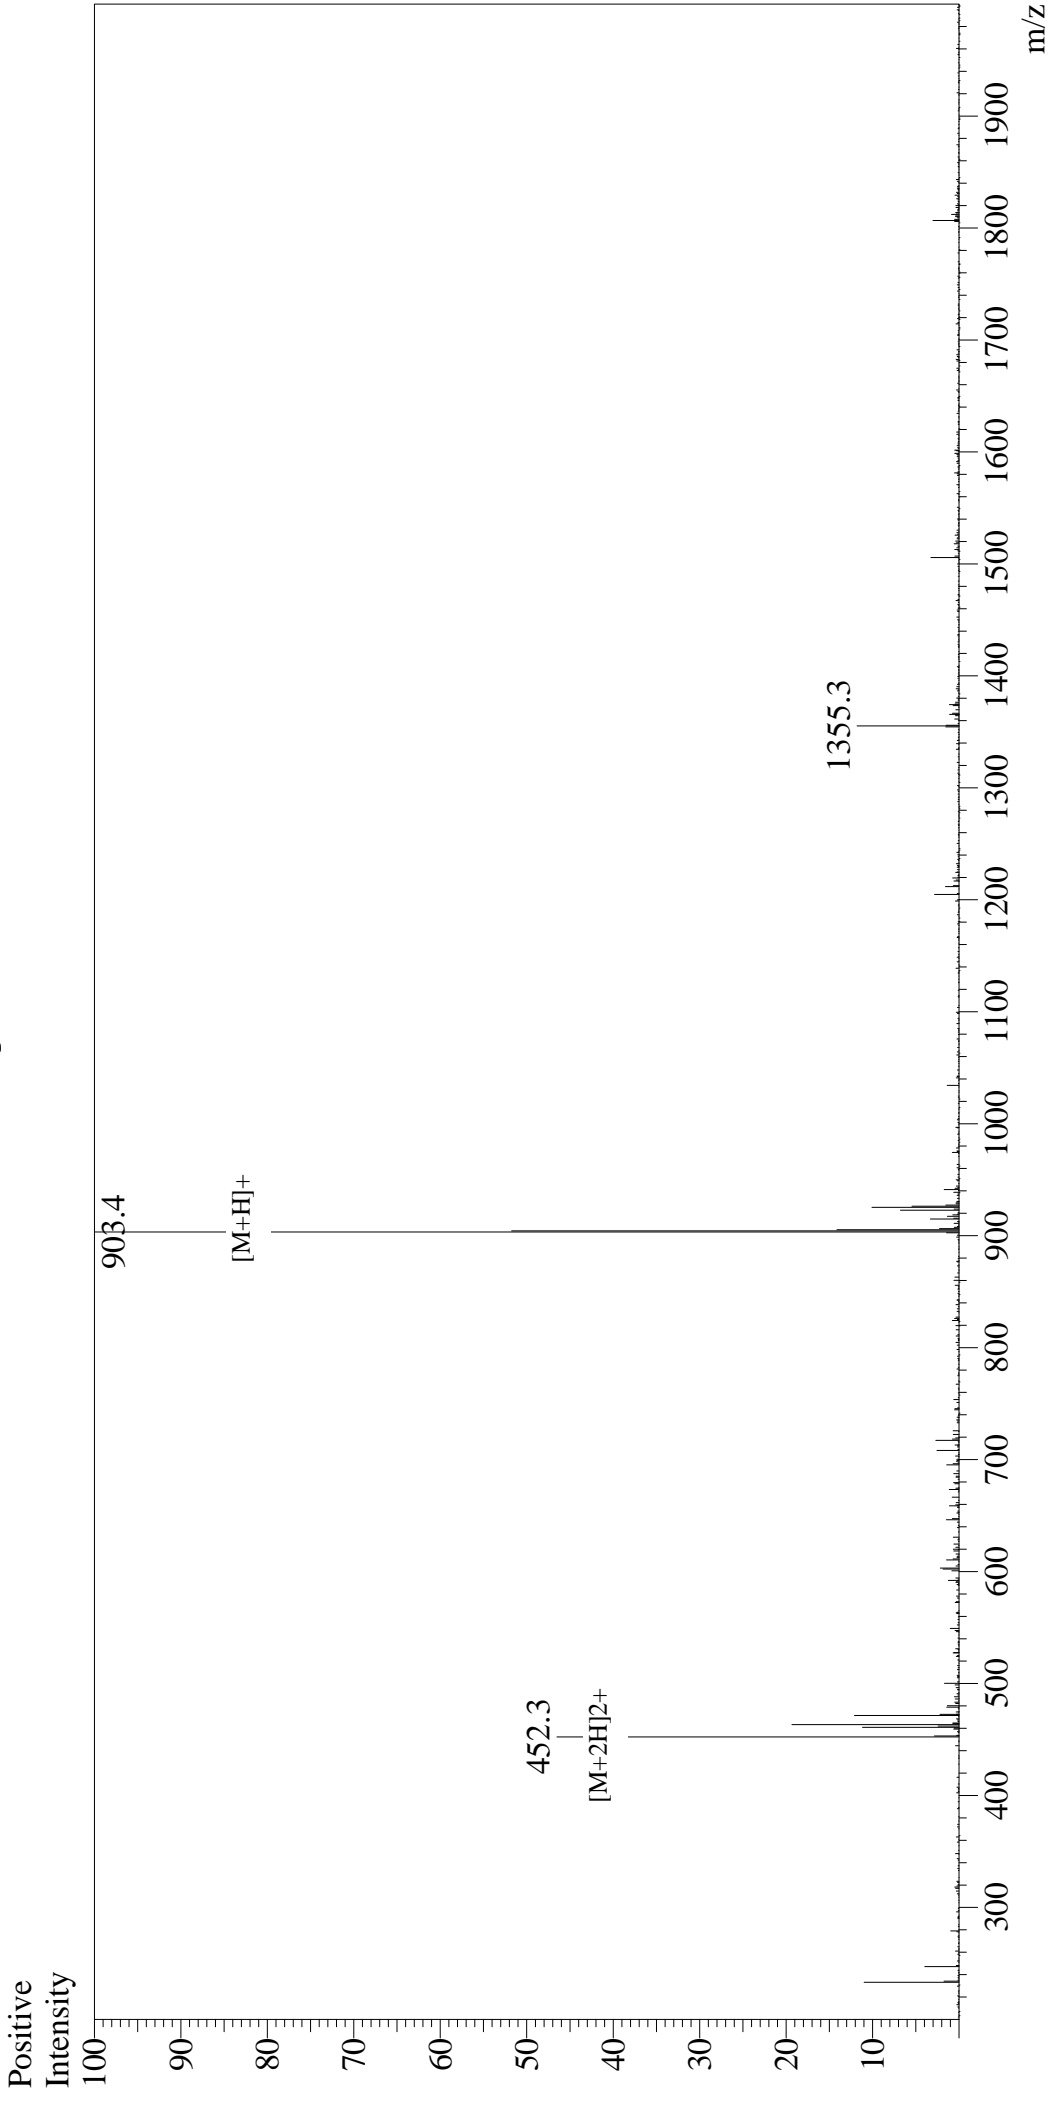

Sample Information

User : Gary
Month-Day Processed : 09/17/19
Time Processed : 22:26:03
Injection Volume : 0.3
Sample Name : Rhodopsin Epitope Tag
Cat No. : RP20400
Lot No. : E4947119I
Theoretical MW : 902.95
Observed MW : 902.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH