

Sample Name : β -Amyloid (25-35)
 Cat No. :RP10008
 Lot No. :E4689119I
 Time Processed :7:49:19
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

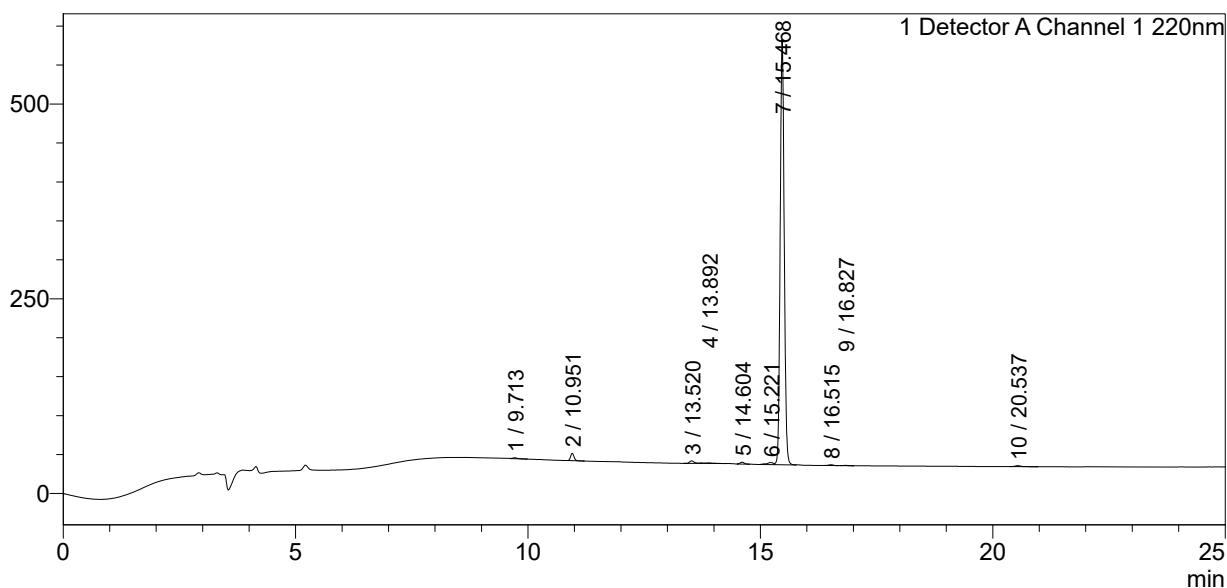

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.713	7872	1114	0.228
2	10.951	48068	9487	1.393
3	13.520	24494	3237	0.710
4	13.892	11061	766	0.320
5	14.604	14807	2366	0.429
6	15.221	26554	2589	0.769
7	15.468	3297103	545993	95.523
8	16.515	7661	1066	0.222
9	16.827	2473	396	0.072
10	20.537	11541	1303	0.334
Total		3451635	568317	100.000