


Sample Name :TAT (48-57)
 Cat. No. : RP20425
 Lot. No. : E7077319J
 Time Processed :7:15:50
 Month-Day-Year Processed : 10/07/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01 | Pumps | Pump A B.Conc | 0 | |
| 5.00 | Pumps | Pump A B.Conc | 0 | |
| 20.00 | Pumps | Pump A B.Conc | 30 | |
| 25.00 | Pumps | Pump A B.Conc | 65 | |
| 25.01 | Pumps | Pump A B.Conc | 95 | |
| 31.00 | Pumps | Pump A B.Conc | 95 | |
| 31.01 | Pumps | Pump A B.Conc | 0 | |
| 40.00 | Pumps | Pump A B.Conc | 0 | |
| 40.01 | Controller | Stop | | |

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0286

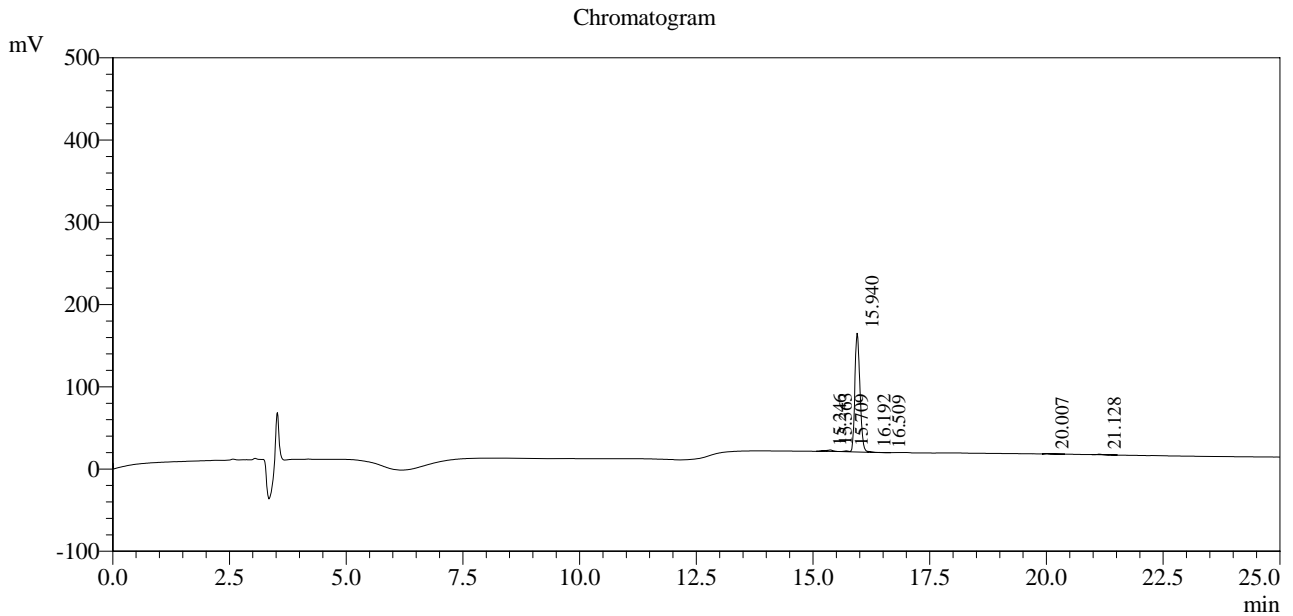

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 15.246 | 8781 | 1124 | 0.771 |
| 2 | 15.363 | 14222 | 1805 | 1.248 |
| 3 | 15.709 | 7541 | 1024 | 0.662 |
| 4 | 15.940 | 1095620 | 144456 | 96.151 |
| 5 | 16.192 | 4465 | 990 | 0.392 |
| 6 | 16.509 | 1082 | 216 | 0.095 |
| 7 | 20.007 | 2479 | 426 | 0.218 |
| 8 | 21.128 | 5292 | 733 | 0.464 |
| Total | | 1139481 | 150774 | 100.000 |