

Sample Name: Cys-TAT(47-57)
 Cat No. : RP20343
 Lot No. : E7988020B
 Time Processed: 8:43:37 AM
 Month-Day-Year Processed :03/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

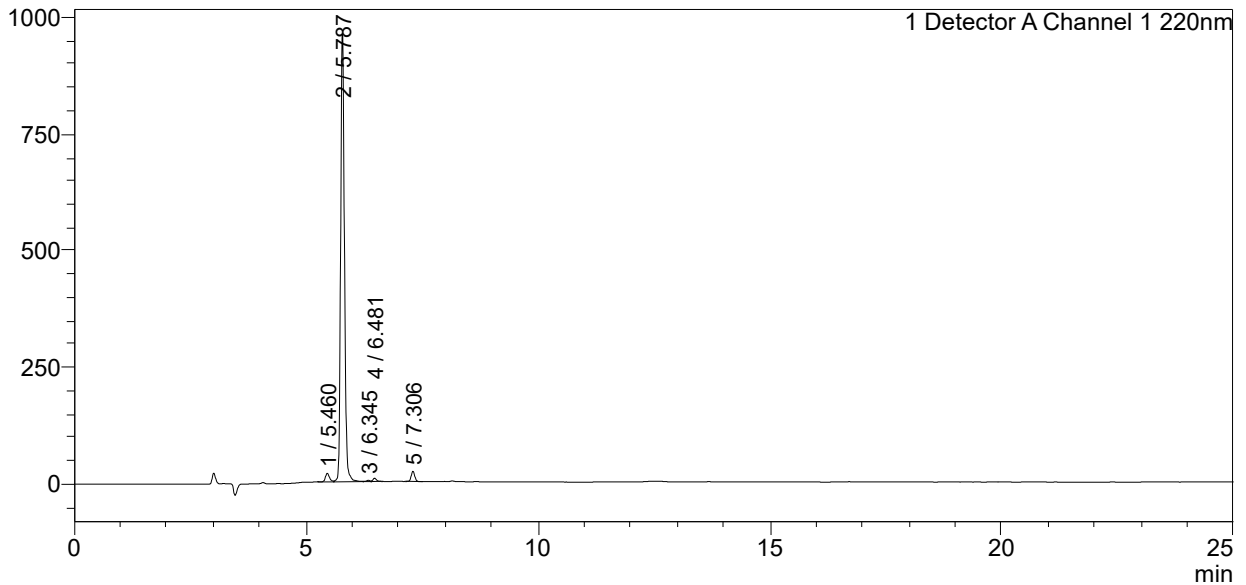

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|---------|---------|
| 1 | 5.460 | 111056 | 18201 | 1.924 |
| 2 | 5.787 | 5497927 | 958992 | 95.246 |
| 3 | 6.345 | 12808 | 2401 | 0.222 |
| 4 | 6.481 | 35468 | 6859 | 0.614 |
| 5 | 7.306 | 115055 | 21791 | 1.993 |
| Total | | 5772315 | 1008243 | 100.000 |