

Sample Name :Galanin Receptor Ligand M35  
 Cat No. :RP10808  
 Lot No. :PE7941902  
 Time Processed :10:35:50  
 Month-Day-Year Processed :03/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command         | Value |
|-------|------------|-----------------|-------|
| 0.01  | Pumps      | Solvent B Conc. | 5     |
| 25.00 | Pumps      | Solvent B Conc. | 65    |
| 25.01 | Pumps      | Solvent B Conc. | 95    |
| 27.00 | Pumps      | Solvent B Conc. | 95    |
| 27.01 | Pumps      | Solvent B Conc. | 5     |
| 33.00 | Pumps      | Solvent B Conc. | 5     |
| 33.01 | Controller | Stop            |       |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

### <Chromatogram>

mV

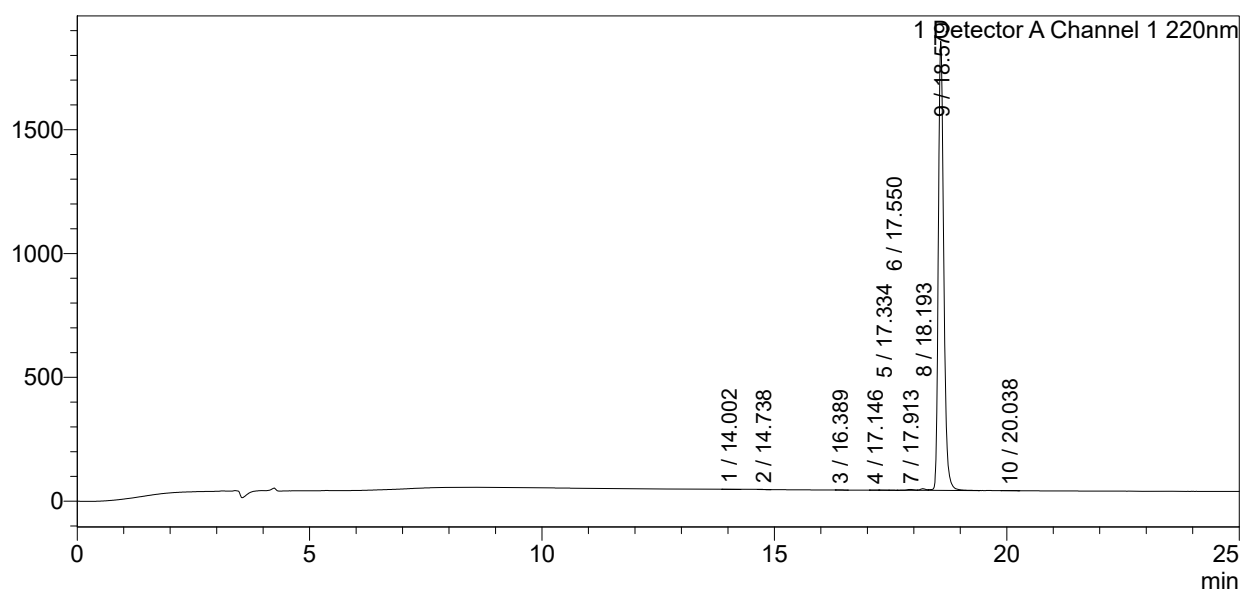

### <Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area     | Height  | Area%   |
|-------|-----------|----------|---------|---------|
| 1     | 14.002    | 8477     | 1120    | 0.057   |
| 2     | 14.738    | 5606     | 924     | 0.038   |
| 3     | 16.389    | 2805     | 384     | 0.019   |
| 4     | 17.146    | 2527     | 368     | 0.017   |
| 5     | 17.334    | 4123     | 519     | 0.028   |
| 6     | 17.550    | 1866     | 277     | 0.013   |
| 7     | 17.913    | 37431    | 3345    | 0.253   |
| 8     | 18.193    | 54886    | 6543    | 0.371   |
| 9     | 18.579    | 14676825 | 1812398 | 99.171  |
| 10    | 20.038    | 4904     | 342     | 0.033   |
| Total |           | 14799452 | 1826220 | 100.000 |