

Sample Name :c-Myc Peptide  
 Cat No. :RP11731  
 Lot No. :E7862621F  
 Time Processed :11:19:37 PM  
 Month-Day-Year Processed :07/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

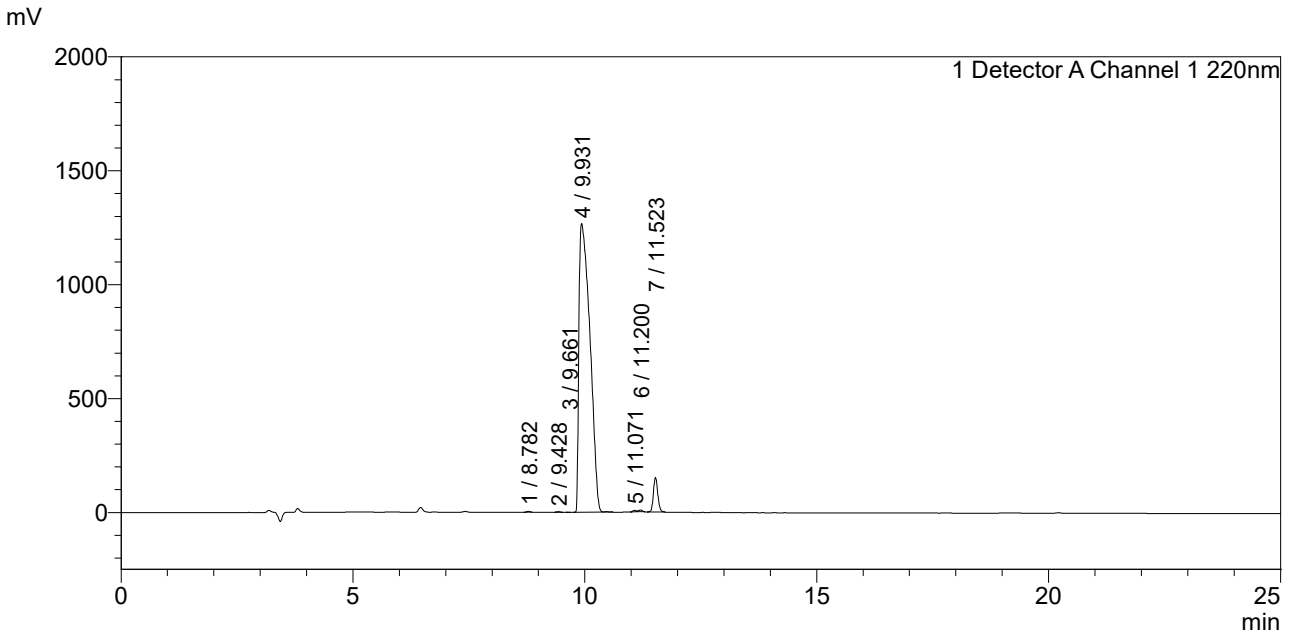

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.782	15223	3276	0.069
2	9.428	11301	2225	0.052
3	9.661	531	61	0.002
4	9.931	20836093	1266803	95.007
5	11.071	34666	6477	0.158
6	11.200	43797	7854	0.200
7	11.523	989432	151460	4.512
Total		21931043	1438156	100.000