

Sample Name :Indolicidin

Cat. No. : RP11242

Lot. No. : PE3741806

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

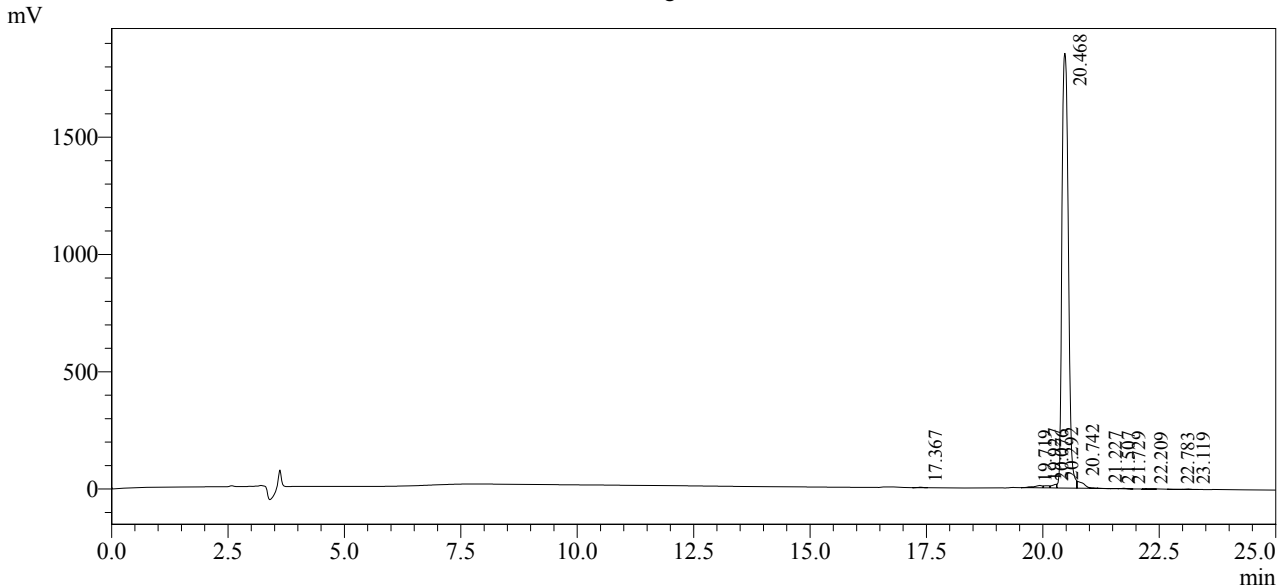

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.367	13191	1872	0.072
2	19.719	28214	3980	0.154
3	19.927	106581	9846	0.581
4	20.076	79344	9181	0.433
5	20.292	106438	15722	0.580
6	20.468	17684637	1853367	96.403
7	20.742	279406	29552	1.523
8	21.227	4897	698	0.027
9	21.507	2208	425	0.012
10	21.729	17432	2050	0.095
11	22.209	5835	914	0.032
12	22.783	4938	621	0.027
13	23.119	11329	1715	0.062
Total		18344451	1929942	100.000