

Sample Name : β -Amyloid (25-35)
 Cat. No. : RP10008 Lot. No. : PE1901810
 Time Processed : 13:41:56
 Month-Day-Year Processed : 10/14/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
32.00	Pumps	Solvent B Conc.	95
32.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

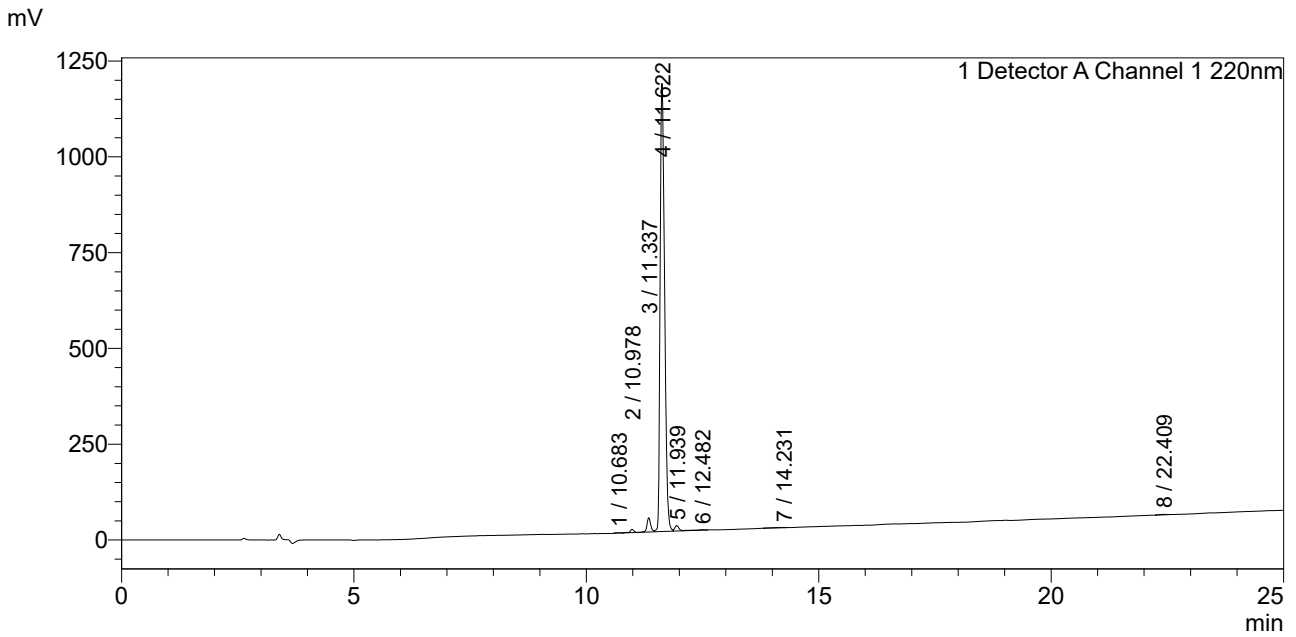

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.683	4659	921	0.057
2	10.978	49047	8427	0.596
3	11.337	209175	37310	2.542
4	11.622	7830031	1169448	95.160
5	11.939	86727	14339	1.054
6	12.482	25158	1271	0.306
7	14.231	10997	343	0.134
8	22.409	12449	1154	0.151
Total		8228243	1233213	100.000